

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Randolph Instrument Location Randolph Co. Jail  
Instrument Serial No. 008899 Asheville, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

655  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

RANDOLPH COUNTY RANDOLPH CO. JAIL 750

Serial Number: 008899

Test Date: 01/09/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2014-11/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

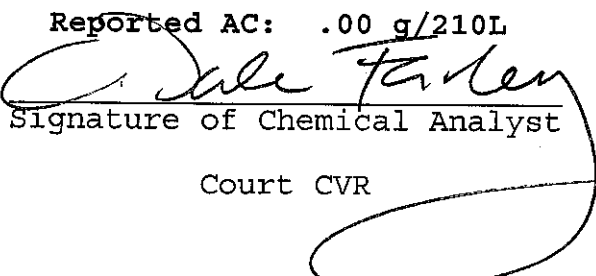
Test Type: Breath Test

Lot Number: AG335201

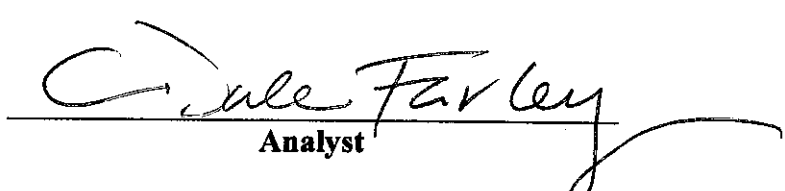
Exp Date: 12/18/2015

| Test            | g/210L     | Time          |
|-----------------|------------|---------------|
| DIAG            | Pass       | 3:48pm        |
| AIR BLK         | .00        | 3:49pm        |
| ACCY CHK        | .07        | 3:49pm        |
| AIR BLK         | .00        | 3:50pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>3:51pm</b> |
| AIR BLK         | .00        | 3:52pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>3:53pm</b> |
| AIR BLK         | .00        | 3:54pm        |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

RANDOLPH COUNTY RANDOLPH CO. JAIL 750

Serial Number: 008899      Test Record Number: 2005

Test Date: 01/09/2015      Test Time: 3:55pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 3:56pm |
| FLO  | Pass   | 3:56pm |
| FC   | Pass   | 3:56pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 3:56pm |
| SRC  | Pass   | 3:56pm |
| DET  | Pass   | 3:56pm |
| BAR  | Pass   | 3:56pm |
| BT   | Pass   | 3:56pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 3:56pm |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 3:56pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 3:57pm |
| CAL  | Pass   | 3:57pm |

Preventive Maintenance  
Status: Pass

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Randolph Instrument Location Randolph Co. Jail  
Instrument Serial No. 008860 Asheboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9<sup>th</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



C. Dale Farley  
Signature of Certifying Official

655  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**RANDOLPH COUNTY RANDOLPH COUNTY JAIL**  
750

Serial Number: 008860  
Test Date: 01/09/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2014-11/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG326006

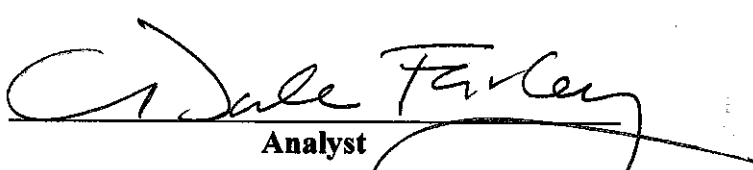
Exp Date: 09/17/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 3:03pm |
| AIR BLK  | .00    | 3:04pm |
| ACCY CHK | .08    | 3:05pm |
| AIR BLK  | .00    | 3:06pm |
| SUB TEST | .00    | 3:06pm |
| AIR BLK  | .00    | 3:07pm |
| SUB TEST | .00    | 3:09pm |
| AIR BLK  | .00    | 3:10pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

**RANDOLPH COUNTY RANDOLPH COUNTY JAIL 750**

Serial Number: 008860      Test Record Number: 2148  
Test Date: 01/09/2015      Test Time: 3:11pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 3:11pm |
| FLO  | Pass   | 3:11pm |
| FC   | Pass   | 3:12pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 3:12pm |
| SRC  | Pass   | 3:12pm |
| DET  | Pass   | 3:12pm |
| BAR  | Pass   | 3:12pm |
| BT   | Pass   | 3:12pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 3:12pm |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 3:12pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 3:13pm |
| CAL  | Pass   | 3:13pm |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County

Randolph

Instrument Location

Randleman P.D.

Instrument Serial No.


008737

Randleman, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9th day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



C. Dale Farley  
Signature of Certifying Official

655  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

RANDOLPH COUNTY RANDLEMAN PD 750

Serial Number: 008737

Test Date: 01/09/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2014-11/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG411202

Exp Date: 04/22/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 12:48pm |
| AIR BLK  | .00    | 12:49pm |
| ACCY CHK | .07    | 12:50pm |
| AIR BLK  | .00    | 12:51pm |
| SUB TEST | .00    | 12:52pm |
| AIR BLK  | .00    | 12:53pm |
| SUB TEST | .00    | 12:54pm |
| AIR BLK  | .00    | 12:55pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007



**Intox EC/IR-II: Preventive Maintenance**

**RANDOLPH COUNTY RANDLEMAN PD 750**

Serial Number: 008737      Test Record Number: 769  
Test Date: 01/09/2015      Test Time: 12:57pm EST

System Check: Passed

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 12:57pm |
| FLO  | Pass   | 12:57pm |
| FC   | Pass   | 12:57pm |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 12:57pm |
| SRC  | Pass   | 12:57pm |
| DET  | Pass   | 12:57pm |
| BAR  | Pass   | 12:57pm |
| BT   | Pass   | 12:57pm |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 12:58pm |

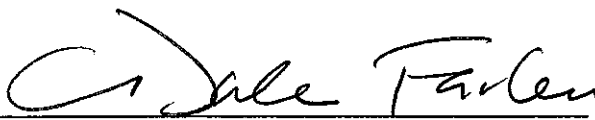
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 12:58pm |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 12:58pm |
| CAL  | Pass   | 12:58pm |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County Durham Instrument Location Durham Co. VA. /  
Instrument Serial No. 008859 217 Mangum St Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of JANUARY, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008859

Test Date: 01/06/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

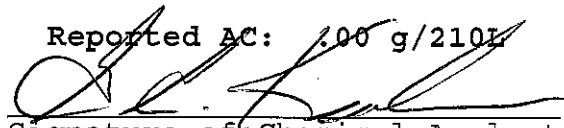
Test Type: Breath Test

Lot Number: AG405702

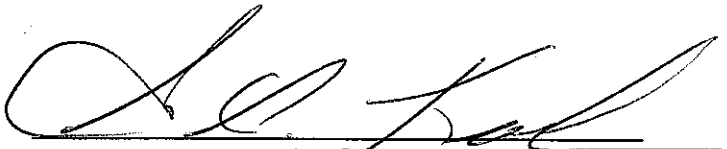
Exp Date: 02/26/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 2:07pm |
| AIR BLK  | .00    | 2:08pm |
| ACCY CHK | .08    | 2:09pm |
| AIR BLK  | .00    | 2:10pm |
| SUB TEST | .00    | 2:11pm |
| AIR BLK  | .00    | 2:12pm |
| SUB TEST | .00    | 2:14pm |
| AIR BLK  | .00    | 2:15pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

*DURHAM COUNTY DURHAM COUNTY JAIL 310*

Serial Number: 008859      Test Record Number: 1847  
Test Date: 01/06/2015      Test Time: 2:16pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 2:16pm |
| FLO  | Pass   | 2:16pm |
| FC   | Pass   | 2:16pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 2:16pm |
| SRC  | Pass   | 2:16pm |
| DET  | Pass   | 2:16pm |
| BAR  | Pass   | 2:16pm |
| BT   | Pass   | 2:16pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 2:17pm |

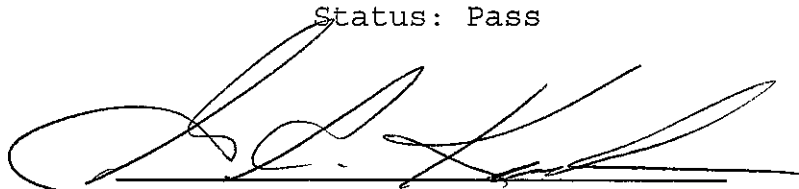
**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 2:17pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 2:17pm |
| CAL  | Pass   | 2:17pm |

Preventive Maintenance  
Status: Pass



**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Durham Instrument Location Durham Co. Jail  
Instrument Serial No. 08891 2115. Maxum St Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008891

Test Date: 01/06/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

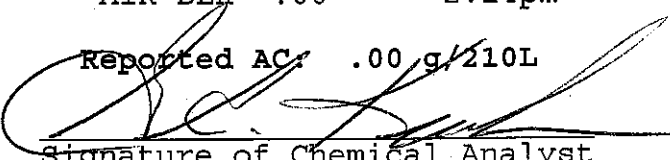
Test Type: Breath Test

Lot Number: AG405702

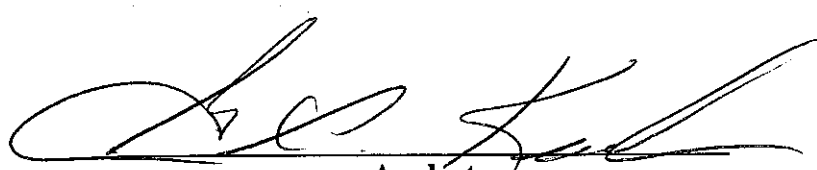
Exp Date: 02/26/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 2:06pm |
| AIR BLK  | .00    | 2:07pm |
| ACCY CHK | .08    | 2:08pm |
| AIR BLK  | .00    | 2:10pm |
| SUB TEST | .00    | 2:10pm |
| AIR BLK  | .00    | 2:11pm |
| SUB TEST | .00    | 2:13pm |
| AIR BLK  | .00    | 2:14pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

**DURHAM COUNTY DURHAM COUNTY JAIL 310**

Serial Number: 008891      Test Record Number: 2806  
Test Date: 01/06/2015      Test Time: 2:15pm EST

System Check: Passed

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 2:16pm |
| FLO  | Pass   | 2:16pm |
| FC   | Pass   | 2:16pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 2:16pm |
| SRC  | Pass   | 2:16pm |
| DET  | Pass   | 2:16pm |
| BAR  | Pass   | 2:16pm |
| BT   | Pass   | 2:16pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 2:16pm |

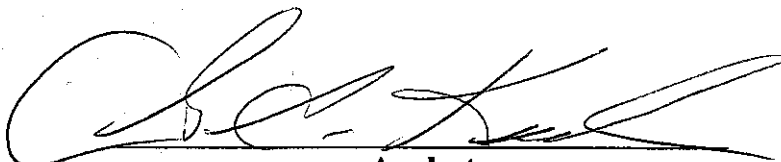
**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 2:17pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 2:17pm |
| CAL  | Pass   | 2:17pm |

Preventive Maintenance  
Status: Pass

  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Durham Instrument Location Durham Co. Jail  
Instrument Serial No. 008818 211 S. Mangum St. Durham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.



**Intox EC/IR-II: Subject Test**

DURHAM COUNTY DURHAM COUNTY JAIL 310

Serial Number: 008878

Test Date: 01/06/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

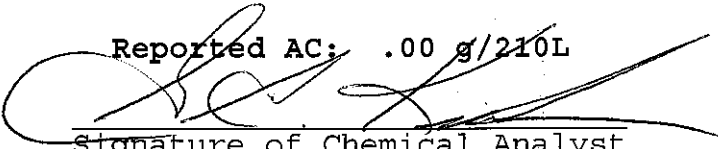
Test Type: Breath Test

Lot Number: AG326006

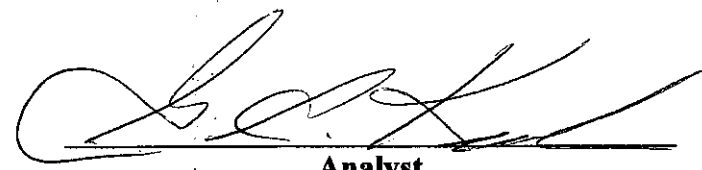
Exp Date: 09/17/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 2:05pm |
| AIR BLK  | .00    | 2:06pm |
| ACCY CHK | .08    | 2:07pm |
| AIR BLK  | .00    | 2:08pm |
| SUB TEST | .00    | 2:09pm |
| AIR BLK  | .00    | 2:10pm |
| SUB TEST | .00    | 2:11pm |
| AIR BLK  | .00    | 2:12pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

**Intox EC/IR-II: Preventive Maintenance**

*DURHAM COUNTY DURHAM COUNTY JAIL 310*

Serial Number: 008878      Test Record Number: 3124

Test Date: 01/06/2015      Test Time: 2:13pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 2:14pm |
| FLO  | Pass   | 2:14pm |
| FC   | Pass   | 2:14pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 2:14pm |
| SRC  | Pass   | 2:14pm |
| DET  | Pass   | 2:14pm |
| BAR  | Pass   | 2:14pm |
| BT   | Pass   | 2:14pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 2:14pm |

**Printer Tests**

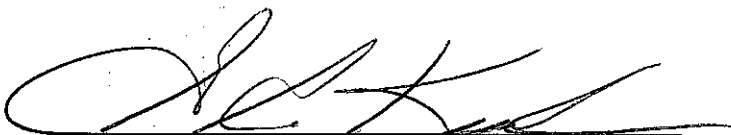
| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 2:14pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 2:15pm |
| CAL  | Pass   | 2:15pm |

Preventive Maintenance

Status: Pass



**Analyst**

**This form is used when performing Preventive Maintenance procedures**

**Forensic Tests for Alcohol Branch**

**Department of Health and Human Services**

**Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Guilford Instrument Location High Point  
Instrument Serial No. 008718 Police Department

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

642  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

GUILFORD COUNTY HIGH POINT PD 401

Serial Number: 008718

Test Date: 01/16/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: DEAN, L K

Permit Number: 11598E

Effective:

06/01/2013-06/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG411202


Exp Date: 04/22/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 1:55pm |
| AIR BLK  | .00    | 1:56pm |
| ACCY CHK | .08    | 1:56pm |
| AIR BLK  | .00    | 1:57pm |
| SUB TEST | .00    | 1:58pm |
| AIR BLK  | .00    | 1:59pm |
| SUB TEST | .00    | 2:00pm |
| AIR BLK  | .00    | 2:01pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**GUILFORD COUNTY HIGH POINT PD 401**

Serial Number: 008718      Test Record Number: 1134  
Test Date: 01/16/2015      Test Time: 1:51pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 1:52pm |
| FLO  | Pass   | 1:52pm |
| FC   | Pass   | 1:52pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 1:52pm |
| SRC  | Pass   | 1:52pm |
| DET  | Pass   | 1:52pm |
| BAR  | Pass   | 1:52pm |
| BT   | Pass   | 1:52pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 1:52pm |


**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 1:53pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 1:53pm |
| CAL  | Pass   | 1:53pm |

Preventive Maintenance  
Status: Pass

  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**


County NASH Instrument Location ROCKY MOUNT PD

Instrument Serial No. 008740 #1 GOVERNMENT PLAZA ROCKY MOUNT, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of JANUARY, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Brian D. Smith  
Signature of Certifying Official

637  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008740      Test Record Number: 523  
Test Date: 01/20/2015      Test Time: 6:52pm EST

System Check: Passed

Baseline Tests

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 6:52pm |
| FLO  | Pass   | 6:52pm |
| FC   | Pass   | 6:52pm |

Temperature Tests

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 6:52pm |
| SRC  | Pass   | 6:52pm |
| DET  | Pass   | 6:52pm |
| BAR  | Pass   | 6:52pm |
| BT   | Pass   | 6:52pm |

Blank Tests

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 6:53pm |


Printer Tests

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 6:53pm |

CRC Tests

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 6:53pm |
| CAL  | Pass   | 6:53pm |

Preventive Maintenance  
Status: Pass



**Analyst**

**Intox EC/IR-II: Subject Test**

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008740

Test Date: 01/20/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SMITH, BRIAN D

Permit Number: 8937E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG409709

Exp Date: 04/07/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 6:44pm |
| AIR BLK  | .00    | 6:45pm |
| ACCY CHK | .08    | 6:45pm |
| AIR BLK  | .00    | 6:46pm |
| SUB TEST | .00    | 6:47pm |
| AIR BLK  | .00    | 6:48pm |
| SUB TEST | .00    | 6:50pm |
| AIR BLK  | .00    | 6:51pm |

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures**

**Forensic Tests for Alcohol Branch**

**Department of Health and Human Services**

**Rev. 12/2007**



DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**


County NASH Instrument Location Rocky Mount PD

Instrument Serial No. 008741 #1 GOVERNMENT PLAZA ROCKY MOUNT, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

637  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

**NASH COUNTY ROCKY MOUNT PD 630**

Serial Number: 008741      Test Record Number: 1607

Test Date: 01/20/2015      Test Time: 6:42pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 6:42pm |
| FLO  | Pass   | 6:42pm |
| FC   | Pass   | 6:42pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 6:42pm |
| SRC  | Pass   | 6:42pm |
| DET  | Pass   | 6:42pm |
| BAR  | Pass   | 6:42pm |
| BT   | Pass   | 6:42pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 6:43pm |


**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 6:43pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 6:43pm |
| CAL  | Pass   | 6:43pm |

Preventive Maintenance  
Status: Pass



**Analyst**

**Intox EC/IR-II: Subject Test**

NASH COUNTY ROCKY MOUNT PD 630

Serial Number: 008741

Test Date: 01/20/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SMITH, BRIAN D

Permit Number: 8937E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG335201

Exp Date: 12/18/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 6:34pm |
| AIR BLK  | .00    | 6:35pm |
| ACCY CHK | .07    | 6:35pm |
| AIR BLK  | .00    | 6:36pm |
| SUB TEST | .00    | 6:37pm |
| AIR BLK  | .00    | 6:38pm |
| SUB TEST | .00    | 6:40pm |
| AIR BLK  | .00    | 6:41pm |

Reported AC: .00 g/210L



Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures**

**Forensic Tests for Alcohol Branch**

**Department of Health and Human Services**

**Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County NASH Instrument Location NASH CO. JAIL

Instrument Serial No. 008630 222 W. WASHINGTON ST. NASHVILLE, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of JANUARY, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bud A. Smith

Signature of Certifying Official

637

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

NASH COUNTY NASH COUNTY JAIL 630

Serial Number: 008630

Test Date: 01/20/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SMITH, BRIAN D

Permit Number: 8937E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG411202


Exp Date: 04/22/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 5:04pm |
| AIR BLK  | .00    | 5:04pm |
| ACCY CHK | .08    | 5:05pm |
| AIR BLK  | .00    | 5:06pm |
| SUB TEST | .00    | 5:07pm |
| AIR BLK  | .00    | 5:08pm |
| SUB TEST | .00    | 5:09pm |
| AIR BLK  | .00    | 5:10pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

NASH COUNTY NASH COUNTY JAIL 630

Serial Number: 008630      Test Record Number: 3267  
Test Date: 01/20/2015      Test Time: 5:13pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 5:13pm |
| FLO  | Pass   | 5:13pm |
| FC   | Pass   | 5:13pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 5:13pm |
| SRC  | Pass   | 5:13pm |
| DET  | Pass   | 5:13pm |
| BAR  | Pass   | 5:13pm |
| BT   | Pass   | 5:13pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 5:14pm |


**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 5:14pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 5:14pm |
| CAL  | Pass   | 5:14pm |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County WAKE Instrument Location APEX P.S. S. #4  
Instrument Serial No. 008621 1615 E. WILLIAMS ST. APEX NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce D. Smith

Signature of Certifying Official

637

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

WAKE COUNTY APEX PD

Serial Number: 008621

Test Date: 01/20/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SMITH, BRIAN D

Permit Number: 8937E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG323402

Exp Date: 08/22/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 2:27pm |
| AIR BLK  | .00    | 2:28pm |
| ACCY CHK | .07    | 2:28pm |
| AIR BLK  | .00    | 2:29pm |
| SUB TEST | .00    | 2:30pm |
| AIR BLK  | .00    | 2:31pm |
| SUB TEST | .00    | 2:32pm |
| AIR BLK  | .00    | 2:33pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst



**Intox EC/IR-II: Preventive Maintenance**

WAKE COUNTY APEX PD

Serial Number: 008621      Test Record Number: 1728

Test Date: 01/20/2015      Test Time: 2:37pm EST

System Check: Passed

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 2:37pm |
| FLO  | Pass   | 2:37pm |
| FC   | Pass   | 2:37pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 2:37pm |
| SRC  | Pass   | 2:37pm |
| DET  | Pass   | 2:37pm |
| BAR  | Pass   | 2:37pm |
| BT   | Pass   | 2:37pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 2:38pm |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 2:38pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 2:39pm |
| CAL  | Pass   | 2:39pm |

Preventive Maintenance  
Status: Pass



**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County VANCE Instrument Location VANCE CO SHERIFF'S OFFICE

Instrument Serial No. 008870 156 CHURCH ST. HENDERSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Brian D. Smith  
Signature of Certifying Official

637  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008870

Test Date: 01/13/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SMITH, BRIAN D

Permit Number: 8937E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG434201

Exp Date: 12/08/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 5:39pm |
| AIR BLK  | .00    | 5:40pm |
| ACCY CHK | .08    | 5:41pm |
| AIR BLK  | .00    | 5:42pm |
| SUB TEST | .00    | 5:43pm |
| AIR BLK  | .00    | 5:44pm |
| SUB TEST | .00    | 5:45pm |
| AIR BLK  | .00    | 5:46pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**VANCE COUNTY SHERIFF'S DEPARTMENT 900**

Serial Number: 008870      Test Record Number: 998

Test Date: 01/13/2015      Test Time: 5:53pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 5:53pm |
| FLO  | Pass   | 5:53pm |
| FC   | Pass   | 5:53pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 5:53pm |
| SRC  | Pass   | 5:53pm |
| DET  | Pass   | 5:53pm |
| BAR  | Pass   | 5:53pm |
| BT   | Pass   | 5:53pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 5:54pm |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 5:54pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 5:54pm |
| CAL  | Pass   | 5:54pm |

Preventive Maintenance  
Status: Pass



**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County VANCE Instrument Location VANCE CO. SHERIFF'S OFFICE  
Instrument Serial No. 008937 156 CHURCH ST. HENDERSON, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce D. Arnold  
Signature of Certifying Official

637  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

VANCE COUNTY SHERIFF'S DEPARTMENT 900

Serial Number: 008937

Test Date: 01/13/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SMITH, BRIAN D

Permit Number: 8937E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG335201

Exp Date: 12/18/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 5:33pm |
| AIR BLK  | .00    | 5:34pm |
| ACCY CHK | .08    | 5:35pm |
| AIR BLK  | .00    | 5:36pm |
| SUB TEST | .00    | 5:36pm |
| AIR BLK  | .00    | 5:37pm |
| SUB TEST | .00    | 5:39pm |
| AIR BLK  | .00    | 5:40pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

**Intox EC/IR-II: Preventive Maintenance**

**VANCE COUNTY SHERIFF'S DEPARTMENT 900**

Serial Number: 008937 Test Record Number: 1674

Test Date: 01/13/2015 Test Time: 5:42pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 5:42pm |
| FLO  | Pass   | 5:42pm |
| FC   | Pass   | 5:42pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 5:42pm |
| SRC  | Pass   | 5:42pm |
| DET  | Pass   | 5:42pm |
| BAR  | Pass   | 5:42pm |
| BT   | Pass   | 5:42pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 5:43pm |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 5:43pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 5:43pm |
| CAL  | Pass   | 5:43pm |

**Preventive Maintenance**

Status: Pass



**Analyst**

**This form is used when performing Preventive Maintenance procedures**

**Forensic Tests for Alcohol Branch**

**Department of Health and Human Services**

**Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Cabarrus


Instrument Location But Mobile Unit 5

Instrument Serial No. 008706

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 9 day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Cell V. Dan  
Signature of Certifying Official

658

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.



Intox EC/IR-II: Subject Test

CABARRUS BAT MOBILE UNIT 5 120

Serial Number: 008706

Test Date: 01/09/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TOWERY, CHAD V

Permit Number: 26632E

Effective:

10/18/2013-10/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

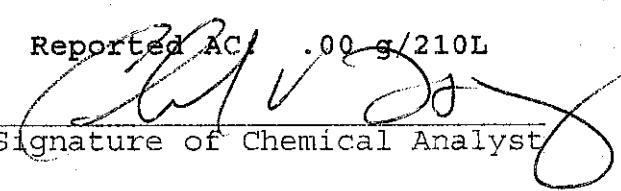
Test Type: Breath Test

Lot Number: AG322601

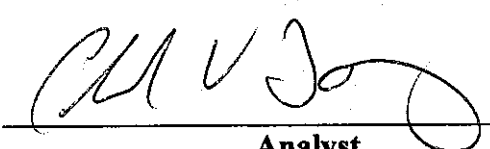
Exp Date: 08/14/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 9:47pm |
| AIR BLK  | .00    | 9:48pm |
| ACCY CHK | .08    | 9:49pm |
| AIR BLK  | .00    | 9:50pm |
| SUB TEST | .00    | 9:50pm |
| AIR BLK  | .00    | 9:51pm |
| SUB TEST | .00    | 9:53pm |
| AIR BLK  | .00    | 9:53pm |

Reported AC/ .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

CABARRUS BAT MOBILE UNIT 5.120

Serial Number: 008706 Test Record Number: 3347

Test Date: 01/09/2015 Test Time: 9:55pm EST

System Check: Passed

Baseline Tests

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 9:55pm |
| FLO  | Pass   | 9:55pm |
| FC   | Pass   | 9:55pm |

Temperature Tests

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 9:55pm |
| SRC  | Pass   | 9:55pm |
| DET  | Pass   | 9:55pm |
| BAR  | Pass   | 9:55pm |
| BT   | Pass   | 9:55pm |

Blank Tests

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 9:56pm |

Printer Tests

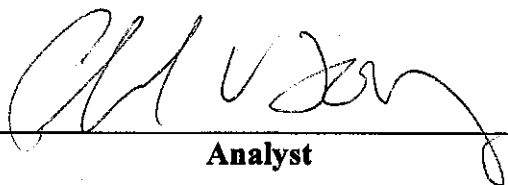
| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 9:56pm |

CRC Tests

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 9:56pm |
| CAL  | Pass   | 9:56pm |

Preventive Maintenance

Status: Pass

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg Instrument Location CMPD-LEC  
Instrument Serial No. 008594 601 E. Trade Street, Charlotte

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7th day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Auhl  
Signature of Certifying Official

650  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

MECKLENBURG COUNTY CMPD LEC 590

Serial Number: 008594

Test Date: 01/07/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

10/01/2013-10/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG418903

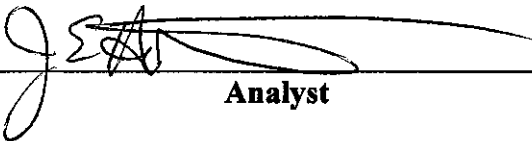
Exp Date: 07/08/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:00am |
| AIR BLK  | .00    | 11:01am |
| ACCY CHK | .07    | 11:02am |
| AIR BLK  | .00    | 11:03am |
| SUB TEST | .00    | 11:03am |
| AIR BLK  | .00    | 11:04am |
| SUB TEST | .00    | 11:06am |
| AIR BLK  | .00    | 11:07am |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

MECKLENBURG COUNTY CPD LEC 590

Serial Number: 008594      Test Record Number: 2456  
Test Date: 01/07/2015      Test Time: 11:08am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:08am |
| FLO  | Pass   | 11:08am |
| FC   | Pass   | 11:08am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:08am |
| SRC  | Pass   | 11:08am |
| DET  | Pass   | 11:08am |
| BAR  | Pass   | 11:08am |
| BT   | Pass   | 11:08am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:09am |


**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:09am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:09am |
| CAL  | Pass   | 11:09am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Iredell Instrument Location Iredell County SD  
Instrument Serial No. 008809 221 E. Water St., Statesville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8<sup>th</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

**IREDELL COUNTY IREDELL COUNTY SD 480**

Serial Number: 008809      Test Record Number: 2826

Test Date: 01/08/2015      Test Time: 8:59am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 9:00am |
| FLO  | Pass   | 9:00am |
| FC   | Pass   | 9:00am |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 9:00am |
| SRC  | Pass   | 9:00am |
| DET  | Pass   | 9:00am |
| BAR  | Pass   | 9:00am |
| BT   | Pass   | 9:00am |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 9:01am |

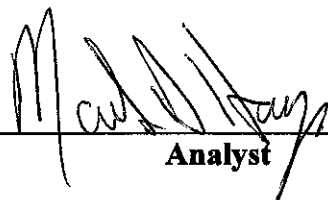
**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 9:01am |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 9:01am |
| CAL  | Pass   | 9:01am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

**Intox EC/IR-II: Subject Test**

IREDELL COUNTY IREDELL COUNTY SD 480

Serial Number: 008809

Test Date: 01/08/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

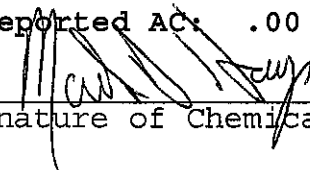
Test Type: Breath Test

Lot Number: AG418903

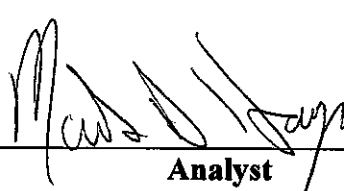
Exp Date: 07/08/2016

| Test            | g/210L     | Time          |
|-----------------|------------|---------------|
| DIAG            | Pass       | 9:04am        |
| AIR BLK         | .00        | 9:04am        |
| ACCY CHK        | .07        | 9:05am        |
| AIR BLK         | .00        | 9:06am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>9:07am</b> |
| AIR BLK         | .00        | 9:08am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>9:10am</b> |
| AIR BLK         | .00        | 9:11am        |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst



DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**


County Iredell Instrument Location Statesville PD

Instrument Serial No. 008619 330 S. Tradd St., Statesville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8<sup>th</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

**IREDELL COUNTY STATESVILLE PD 480**

Serial Number: 008619      Test Record Number: 1064  
Test Date: 01/08/2015      Test Time: 9:25am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 9:26am |
| FLO  | Pass   | 9:26am |
| FC   | Pass   | 9:26am |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 9:26am |
| SRC  | Pass   | 9:26am |
| DET  | Pass   | 9:26am |
| BAR  | Pass   | 9:26am |
| BT   | Pass   | 9:26am |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 9:27am |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 9:27am |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 9:27am |
| CAL  | Pass   | 9:27am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
Analyst

**Intox EC/IR-II: Subject Test**

**IREDELL COUNTY STATESVILLE PD 480**

Serial Number: 008619

Test Date: 01/08/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

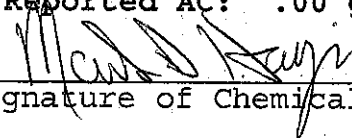
Test Type: Breath Test

Lot Number: AG308702

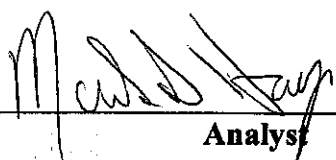
Exp Date: 03/28/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 9:29am |
| AIR BLK  | .00    | 9:30am |
| ACCY CHK | .08    | 9:30am |
| AIR BLK  | .00    | 9:31am |
| SUB TEST | .00    | 9:32am |
| AIR BLK  | .00    | 9:33am |
| SUB TEST | .00    | 9:35am |
| AIR BLK  | .00    | 9:36am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Iredell Instrument Location Mooreville PD  
Instrument Serial No. 008685 750 W. Iredell Ave, Mooreville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8<sup>th</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Preventive Maintenance

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685      Test Record Number: 2310  
Test Date: 01/08/2015      Test Time: 10:16am EST

System Check: Passed

Baseline Tests

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:17am |
| FLO  | Pass   | 10:17am |
| FC   | Pass   | 10:17am |

Temperature Tests

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:17am |
| SRC  | Pass   | 10:17am |
| DET  | Pass   | 10:17am |
| BAR  | Pass   | 10:17am |
| BT   | Pass   | 10:17am |

Blank Tests

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:18am |

Printer Tests

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:18am |

CRC Tests

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:18am |
| CAL  | Pass   | 10:18am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
Analyst

Intox EC/IR-II: Subject Test

IREDELL COUNTY MOORESVILLE PD 480

Serial Number: 008685

Test Date: 01/08/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

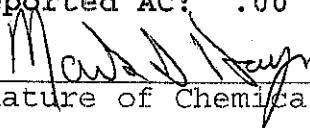
Test Type: Breath Test

Lot Number: AG425303

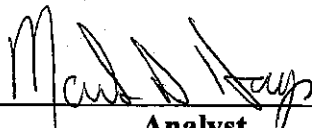
Exp Date: 09/10/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:29am |
| AIR BLK  | .00    | 10:30am |
| ACCY CHK | .07    | 10:30am |
| AIR BLK  | .00    | 10:31am |
| SUB TEST | .00    | 10:32am |
| AIR BLK  | .00    | 10:33am |
| SUB TEST | .00    | 10:34am |
| AIR BLK  | .00    | 10:35am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Cleveland Instrument Location Cleveland County SD  
Instrument Serial No. 008893 100 Justice Place, Shelby

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12<sup>th</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M. A. D. [Signature]  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

**CLEVELAND COUNTY CLEVELAND COUNTY SD 220**

Serial Number: 008893      Test Record Number: 1284  
Test Date: 01/12/2015      Test Time: 9:40am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 9:40am |
| FLO  | Pass   | 9:40am |
| FC   | Pass   | 9:40am |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 9:40am |
| SRC  | Pass   | 9:40am |
| DET  | Pass   | 9:40am |
| BAR  | Pass   | 9:40am |
| BT   | Pass   | 9:40am |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 9:41am |

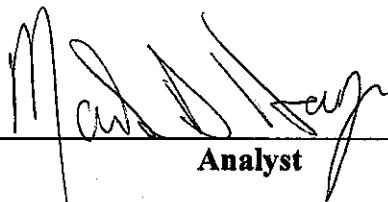
**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 9:41am |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 9:41am |
| CAL  | Pass   | 9:41am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**



Intox EC/IR-II: Subject Test

CLEVELAND COUNTY CLEVELAND COUNTY SD  
220

Serial Number: 008893  
Test Date: 01/12/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

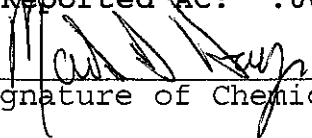
Test Type: Breath Test

Lot Number: AG320602

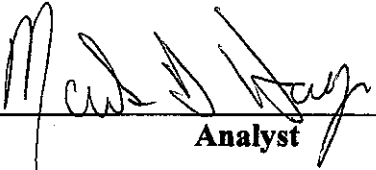
Exp Date: 07/25/2015

| Test            | g/210L     | Time          |
|-----------------|------------|---------------|
| DIAG            | Pass       | 9:45am        |
| AIR BLK         | .00        | 9:45am        |
| ACCY CHK        | .08        | 9:46am        |
| AIR BLK         | .00        | 9:47am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>9:48am</b> |
| AIR BLK         | .00        | 9:49am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>9:50am</b> |
| AIR BLK         | .00        | 9:51am        |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Cleveland Instrument Location Cleveland County SD Annex  
Instrument Serial No. 008887 407 McBrayer St., Shelby

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12<sup>th</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

**CLEVELAND COUNTY CLEVELAND SD-ANNEX 220**

Serial Number: 008887      Test Record Number: 1943  
Test Date: 01/12/2015      Test Time: 10:17am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:18am |
| FLO  | Pass   | 10:18am |
| FC   | Pass   | 10:18am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:18am |
| SRC  | Pass   | 10:18am |
| DET  | Pass   | 10:18am |
| BAR  | Pass   | 10:18am |
| BT   | Pass   | 10:18am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:19am |

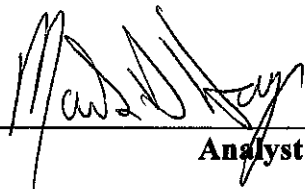
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:19am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:19am |
| CAL  | Pass   | 10:19am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

**Intox EC/IR-II: Subject Test**

**CLEVELAND COUNTY CLEVELAND SD-ANNEX**  
220

Serial Number: 008887

Test Date: 01/12/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

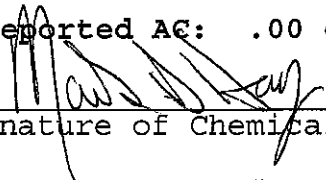
Test Type: Breath Test

Lot Number: AG326006

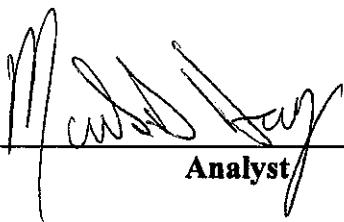
Exp Date: 09/17/2015

| Test            | g/210L     | Time           |
|-----------------|------------|----------------|
| DIAG            | Pass       | 10:23am        |
| AIR BLK         | .00        | 10:24am        |
| ACCY CHK        | .08        | 10:25am        |
| AIR BLK         | .00        | 10:26am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>10:26am</b> |
| AIR BLK         | .00        | 10:27am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>10:29am</b> |
| AIR BLK         | .00        | 10:30am        |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

**This form is used when performing Preventive Maintenance procedures**  
**Forensic Tests for Alcohol Branch**  
**Department of Health and Human Services**  
**Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wayne Instrument Location Wayne Co. Detention ctr.  
Instrument Serial No. 008649 207 E. Churston St., Goldsboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12<sup>th</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Lincoln A. Kersh  
Signature of Certifying Official

647  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008649

Test Date: 01/12/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A

Permit Number: 11646E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG315701


Exp Date: 06/06/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 12:41pm |
| AIR BLK  | .00    | 12:42pm |
| ACCY CHK | .07    | 12:43pm |
| AIR BLK  | .00    | 12:44pm |
| SUB TEST | .00    | 12:45pm |
| AIR BLK  | .00    | 12:45pm |
| SUB TEST | .00    | 12:47pm |
| AIR BLK  | .00    | 12:48pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008649 Test Record Number: 2614

Test Date: 01/12/2015 Test Time: 12:49pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 12:49pm |
| FLO  | Pass   | 12:49pm |
| FC   | Pass   | 12:50pm |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 12:50pm |
| SRC  | Pass   | 12:50pm |
| DET  | Pass   | 12:50pm |
| BAR  | Pass   | 12:50pm |
| BT   | Pass   | 12:50pm |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 12:50pm |


**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 12:50pm |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 12:50pm |
| CAL  | Pass   | 12:50pm |

Preventive Maintenance  
Status: Pass



**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County Mecklenburg Instrument Location Matthews PD  
Instrument Serial No. 008699 1201 Crews Rd., Matthews

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16<sup>th</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M. J. Hays  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.



**Intox EC/IR-II: Preventive Maintenance**

**MECKLENBURG COUNTY MATTHEWS PD 590**

Serial Number: 008699      Test Record Number: 2244

Test Date: 01/16/2015      Test Time: 11:34am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:35am |
| FLO  | Pass   | 11:35am |
| FC   | Pass   | 11:35am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:35am |
| SRC  | Pass   | 11:35am |
| DET  | Pass   | 11:35am |
| BAR  | Pass   | 11:35am |
| BT   | Pass   | 11:35am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:36am |

**Printer Tests**

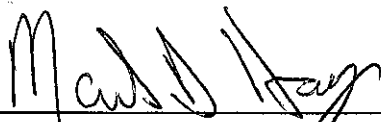
| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:36am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:36am |
| CAL  | Pass   | 11:36am |

**Preventive Maintenance**

Status: Pass

  
\_\_\_\_\_  
**Analyst**

**Intox EC/IR-II: Subject Test**

**MECKLENBURG COUNTY MATTHEWS PD 590**

Serial Number: 008699

Test Date: 01/16/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

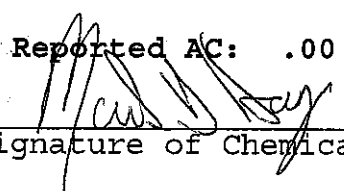
Test Type: Breath Test

Lot Number: AG326006

Exp Date: 09/17/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:39am |
| AIR BLK  | .00    | 11:40am |
| ACCY CHK | .08    | 11:41am |
| AIR BLK  | .00    | 11:42am |
| SUB TEST | .00    | 11:43am |
| AIR BLK  | .00    | 11:44am |
| SUB TEST | .00    | 11:45am |
| AIR BLK  | .00    | 11:46am |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg Instrument Location Pineville PD  
Instrument Serial No. 008703 427 Main St, Pineville

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16<sup>th</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



M. A. Hagan  
Signature of Certifying Official

056  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

**MECKLENBURG COUNTY PINEVILLE PD 590**

Serial Number: 008703      Test Record Number: 5348  
Test Date: 01/16/2015      Test Time: 10:33am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:34am |
| FLO  | Pass   | 10:34am |
| FC   | Pass   | 10:34am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:34am |
| SRC  | Pass   | 10:34am |
| DET  | Pass   | 10:34am |
| BAR  | Pass   | 10:34am |
| BT   | Pass   | 10:34am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:35am |

**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:35am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:35am |
| CAL  | Pass   | 10:35am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
Analyst

**Intox EC/IR-II: Subject Test**

**MECKLENBURG COUNTY PINEVILLE PD 590**

Serial Number: 008703

Test Date: 01/16/2015

Citation Number: M0000000-0

Subject's Name:

**PREVENTIVE, MAINTENANCE**

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

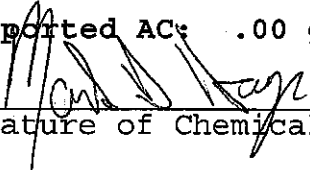
Test Type: Breath Test

Lot Number: AG335201

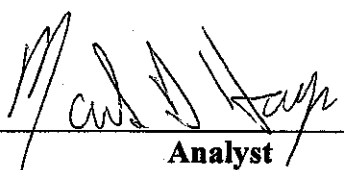
Exp Date: 12/18/2015

| Test            | g/210L     | Time           |
|-----------------|------------|----------------|
| DIAG            | Pass       | 10:38am        |
| AIR BLK         | .00        | 10:39am        |
| ACCY CHK        | .08        | 10:39am        |
| AIR BLK         | .00        | 10:40am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>10:41am</b> |
| AIR BLK         | .00        | 10:41am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>10:43am</b> |
| AIR BLK         | .00        | 10:44am        |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg Instrument Location Mecklenburg County SD  
Instrument Serial No. 008690 801 E. 4<sup>th</sup> St. Charlotte

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20<sup>th</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

**MECKLENBURG COUNTY SHERIFFS DEPARTMENT 590**

Serial Number: 008690      Test Record Number: 4695  
Test Date: 01/20/2015      Test Time: 10:31am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:32am |
| FLO  | Pass   | 10:32am |
| FC   | Pass   | 10:32am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:32am |
| SRC  | Pass   | 10:32am |
| DET  | Pass   | 10:32am |
| BAR  | Pass   | 10:32am |
| BT   | Pass   | 10:32am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:33am |

**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:33am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:33am |
| CAL  | Pass   | 10:33am |

Preventive Maintenance  
Status: *Pass*

  
\_\_\_\_\_  
**Analyst**

**Intox EC/IR-II: Subject Test**

MECKLENBURG COUNTY SHERIFFS DEPARTMENT  
590

Serial Number: 008690

Test Date: 01/20/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

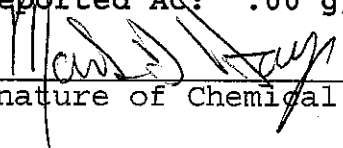
Test Type: Breath Test

Lot Number: AG425303

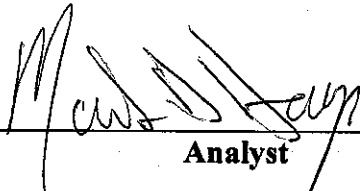
Exp Date: 09/10/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:44am |
| AIR BLK  | .00    | 10:45am |
| ACCY CHK | .08    | 10:46am |
| AIR BLK  | .00    | 10:47am |
| SUB TEST | .00    | 10:48am |
| AIR BLK  | .00    | 10:49am |
| SUB TEST | .00    | 10:50am |
| AIR BLK  | .00    | 10:51am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007



DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Lincoln Instrument Location Lincoln County Courthouse  
Instrument Serial No. 008823 #1 Courthouse Square, Lincolnton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21<sup>st</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark D. Hay  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

LINCOLN COUNTY COURTHOUSE 540

Serial Number: 008823

Test Date: 01/21/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG404101


Exp Date: 02/10/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 9:51am |
| AIR BLK  | .00    | 9:52am |
| ACCY CHK | .07    | 9:53am |
| AIR BLK  | .00    | 9:54am |
| SUB TEST | .00    | 9:54am |
| AIR BLK  | .00    | 9:56am |
| SUB TEST | .00    | 9:57am |
| AIR BLK  | .00    | 9:58am |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**LINCOLN COUNTY COURTHOUSE 540**

Serial Number: 008823      Test Record Number: 1144  
Test Date: 01/21/2015      Test Time: 9:46am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 9:47am |
| FLO  | Pass   | 9:47am |
| FC   | Pass   | 9:47am |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 9:47am |
| SRC  | Pass   | 9:47am |
| DET  | Pass   | 9:47am |
| BAR  | Pass   | 9:47am |
| BT   | Pass   | 9:47am |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 9:48am |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 9:48am |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 9:48am |
| CAL  | Pass   | 9:48am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Rutherford Instrument Location Rutherford County SD  
Instrument Serial No. 008914 400 N. Washington St., Rutherfordton

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22<sup>nd</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mark D. Hays  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

*RUTHERFORD COUNTY RUTHERFORD COUNTY SD 800*

Serial Number: 008914      Test Record Number: 1543  
Test Date: 01/22/2015      Test Time: 10:30am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:30am |
| FLO  | Pass   | 10:30am |
| FC   | Pass   | 10:31am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:31am |
| SRC  | Pass   | 10:31am |
| DET  | Pass   | 10:31am |
| BAR  | Pass   | 10:31am |
| BT   | Pass   | 10:31am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:31am |

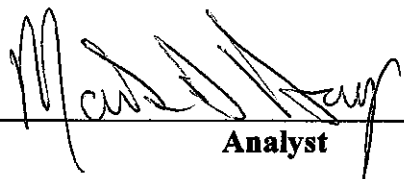
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:31am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:31am |
| CAL  | Pass   | 10:31am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

**Intox EC/IR-II: Subject Test**

RUTHERFORD COUNTY RUTHERFORD COUNTY SD  
800

Serial Number: 008914

Test Date: 01/22/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG309101


Exp Date: 04/01/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:34am |
| AIR BLK  | .00    | 10:34am |
| ACCY CHK | .07    | 10:35am |
| AIR BLK  | .00    | 10:36am |
| SUB TEST | .00    | 10:37am |
| AIR BLK  | .00    | 10:38am |
| SUB TEST | .00    | 10:40am |
| AIR BLK  | .00    | 10:41am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Polk Instrument Location Polk County SD  
Instrument Serial No. 008832 46 Ward St., Columbus

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Mads A. Hansen  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

POLK COUNTY POLK COUNTY SD 740

Serial Number: 008832      Test Record Number: 1125  
Test Date: 01/22/2015      Test Time: 11:38am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:39am |
| FLO  | Pass   | 11:39am |
| FC   | Pass   | 11:39am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:39am |
| SRC  | Pass   | 11:39am |
| DET  | Pass   | 11:39am |
| BAR  | Pass   | 11:39am |
| BT   | Pass   | 11:39am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:40am |

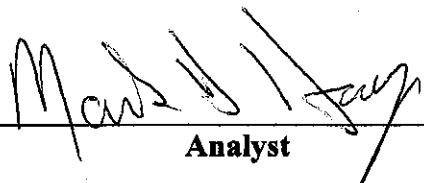
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:40am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:40am |
| CAL  | Pass   | 11:40am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**



**Intox EC/IR-II: Subject Test**

POLK COUNTY POLK COUNTY SD 740

Serial Number: 008832

Test Date: 01/22/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HAYS, MARK D

Permit Number: 15924E

Effective:

01/01/2014-01/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

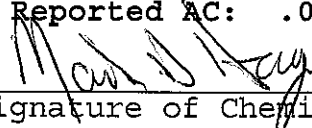
Test Type: Breath Test

Lot Number: AG309101

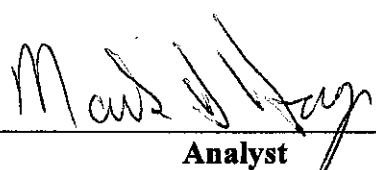
Exp Date: 04/01/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:43am |
| AIR BLK  | .00    | 11:43am |
| ACCY CHK | .07    | 11:44am |
| AIR BLK  | .00    | 11:45am |
| SUB TEST | .00    | 11:45am |
| AIR BLK  | .00    | 11:46am |
| SUB TEST | .00    | 11:48am |
| AIR BLK  | .00    | 11:49am |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Martin Instrument Location Martin Co. S.O.

Instrument Serial No. 008912 305 E. Main St., Williamston, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23<sup>rd</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kelly M. O.  
Signature of Certifying Official

643  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

MARTIN COUNTY SHERIFF'S OFFICE 570

Serial Number: 008912

Test Date: 01/23/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG309105


Exp Date: 04/01/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:27am |
| AIR BLK  | .00    | 10:27am |
| ACCY CHK | .08    | 10:28am |
| AIR BLK  | .00    | 10:29am |
| SUB TEST | .00    | 10:30am |
| AIR BLK  | .00    | 10:31am |
| SUB TEST | .00    | 10:32am |
| AIR BLK  | .00    | 10:33am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**MARTIN COUNTY SHERIFF'S OFFICE 570**

Serial Number: 008912      Test Record Number: 927  
Test Date: 01/23/2015      Test Time: 10:35am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:35am |
| FLO  | Pass   | 10:35am |
| FC   | Pass   | 10:35am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:35am |
| SRC  | Pass   | 10:35am |
| DET  | Pass   | 10:35am |
| BAR  | Pass   | 10:35am |
| BT   | Pass   | 10:35am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:36am |

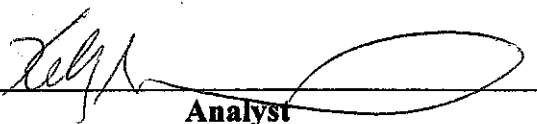
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:36am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:36am |
| CAL  | Pass   | 10:36am |

Preventive Maintenance  
Status: Pass

  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Chowan Instrument Location Chowan Co. Public Safety Center  
Instrument Serial No. 008895 305 W. Freemason St., Edenboro, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kelly A. [Signature]  
Signature of Certifying Official

643  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**CHOWAN COUNTY PUBLIC SAFETY CENTER 200**

Serial Number: 008895

Test Date: 01/22/2015

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG315701

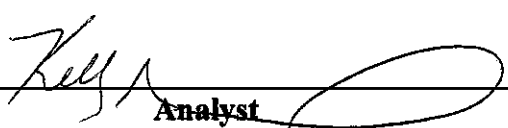
Exp Date: 06/06/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:38am |
| AIR BLK  | .00    | 10:39am |
| ACCY CHK | .07    | 10:40am |
| AIR BLK  | .00    | 10:41am |
| SUB TEST | .00    | 10:43am |
| AIR BLK  | .00    | 10:43am |
| SUB TEST | .00    | 10:46am |
| AIR BLK  | .00    | 10:47am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

CHOWAN COUNTY PUBLIC SAFETY CENTER 200

Serial Number: 008895      Test Record Number: 648  
Test Date: 01/22/2015      Test Time: 11:13am EST

System Check: Passed

Baseline Tests

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:13am |
| FLO  | Pass   | 11:13am |
| FC   | Pass   | 11:14am |

Temperature Tests

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:14am |
| SRC  | Pass   | 11:14am |
| DET  | Pass   | 11:14am |
| BAR  | Pass   | 11:14am |
| BT   | Pass   | 11:14am |

Blank Tests

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:14am |

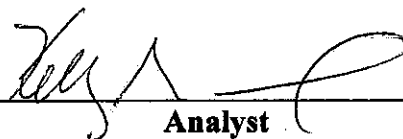
Printer Tests

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:14am |

CRC Tests

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:15am |
| CAL  | Pass   | 11:15am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Pitt Instrument Location Pitt Co. Detention Center  
Instrument Serial No. 008662 124 Detention Dr., Greenville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21<sup>st</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Kelly S. P.

Signature of Certifying Official

643

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.



**Intox EC/IR-II: Subject Test**

PITT COUNTY PITT CO DETENTION 730

Serial Number: 008662

Test Date: 01/21/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

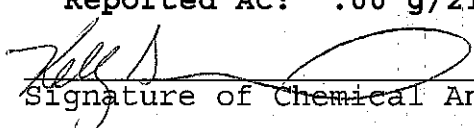
Test Type: Breath Test

Lot Number: AG400603

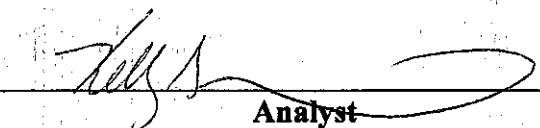
Exp Date: 01/06/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:16am |
| AIR BLK  | .00    | 10:17am |
| ACCY CHK | .07    | 10:17am |
| AIR BLK  | .00    | 10:18am |
| SUB TEST | .00    | 10:19am |
| AIR BLK  | .00    | 10:20am |
| SUB TEST | .00    | 10:21am |
| AIR BLK  | .00    | 10:22am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**PITT COUNTY PITT CO DETENTION 730**

Serial Number: 008662      Test Record Number: 841  
Test Date: 01/21/2015      Test Time: 10:23am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:23am |
| FLO  | Pass   | 10:24am |
| FC   | Pass   | 10:24am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:24am |
| SRC  | Pass   | 10:24am |
| DET  | Pass   | 10:24am |
| BAR  | Pass   | 10:24am |
| BT   | Pass   | 10:24am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:24am |

**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:24am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:25am |
| CAL  | Pass   | 10:25am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Pitt Instrument Location Pitt Co. Detention Center  
Instrument Serial No. 0086608 124 Detention Dr., Greenville, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 21<sup>st</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

643  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**PITT COUNTY PITT CO DETENTION 730**

Serial Number: 008668

Test Date: 01/21/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONF

Analyst's Name: GUARD, KELLY G

Permit Number: 12955E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG414801

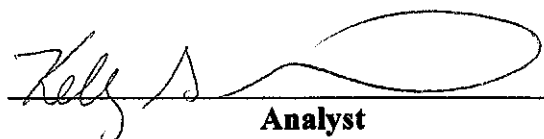
Exp Date: 05/28/2016

| Test            | g/210L     | Time           |
|-----------------|------------|----------------|
| DIAG            | Pass       | 9:56am         |
| AIR BLK         | .00        | 9:57am         |
| ACCY CHK        | .08        | 9:58am         |
| AIR BLK         | .00        | 9:59am         |
| <b>SUB TEST</b> | <b>.00</b> | <b>9:59am</b>  |
| AIR BLK         | .00        | 10:00am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>10:02am</b> |
| AIR BLK         | .00        | 10:03am        |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**PITT COUNTY PITT CO DETENTION 730**

Serial Number: 008668      Test Record Number: 2501

Test Date: 01/21/2015      Test Time: 10:03am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:04am |
| FLO  | Pass   | 10:04am |
| FC   | Pass   | 10:04am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:04am |
| SRC  | Pass   | 10:04am |
| DET  | Pass   | 10:04am |
| BAR  | Pass   | 10:04am |
| BT   | Pass   | 10:04am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:05am |

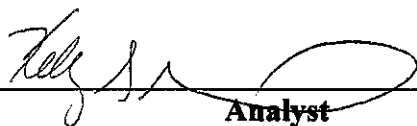
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:05am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:05am |
| CAL  | Pass   | 10:05am |

Preventive Maintenance  
Status: Pass

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County WAKE Instrument Location WAKE CO DETENTION CENTER

Instrument Serial No. 008651 3301 HAMMOND RD RALEIGH, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Bruce D. Smith  
Signature of Certifying Official

637  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008651

Test Date: 01/22/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: SMITH, BRIAN D

Permit Number: 8937E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG425303

Exp Date: 09/10/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 5:04pm |
| AIR BLK  | .00    | 5:05pm |
| ACCY CHK | .08    | 5:06pm |
| AIR BLK  | .00    | 5:07pm |
| SUB TEST | .00    | 5:07pm |
| AIR BLK  | .00    | 5:08pm |
| SUB TEST | .00    | 5:10pm |
| AIR BLK  | .00    | 5:10pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008651      Test Record Number: 1059  
Test Date: 01/22/2015      Test Time: 5:13pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 5:13pm |
| FLO  | Pass   | 5:13pm |
| FC   | Pass   | 5:13pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 5:13pm |
| SRC  | Pass   | 5:13pm |
| DET  | Pass   | 5:13pm |
| BAR  | Pass   | 5:13pm |
| BT   | Pass   | 5:13pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 5:14pm |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 5:14pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 5:14pm |
| CAL  | Pass   | 5:14pm |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
Analyst



DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Alamance Instrument Location Burlington P.D.  
Instrument Serial No. 008812 257 W. Front St.  
Burlington, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

ALAMANCE COUNTY BURLINGTON PD 000

Serial Number: 008812

Test Date: 01/06/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

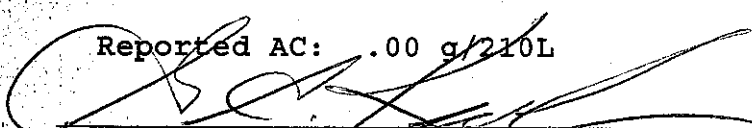
Test Type: Breath Test

Lot Number: AG326006

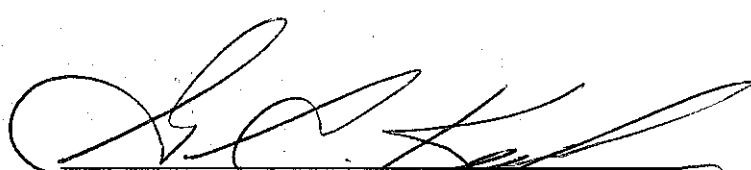
Exp Date: 09/17/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:27am |
| AIR BLK  | .00    | 10:28am |
| ACCY CHK | .07    | 10:28am |
| AIR BLK  | .00    | 10:29am |
| SUB TEST | .00    | 10:30am |
| AIR BLK  | .00    | 10:31am |
| SUB TEST | .00    | 10:33am |
| AIR BLK  | .00    | 10:34am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

**ALAMANCE COUNTY BURLINGTON PD 000**

Serial Number: 008812      Test Record Number: 2203  
Test Date: 01/06/2015      Test Time: 10:36am EST

System Check: Passed

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:36am |
| FLO  | Pass   | 10:36am |
| FC   | Pass   | 10:36am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:37am |
| SRC  | Pass   | 10:37am |
| DET  | Pass   | 10:37am |
| BAR  | Pass   | 10:37am |
| BT   | Pass   | 10:37am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:37am |

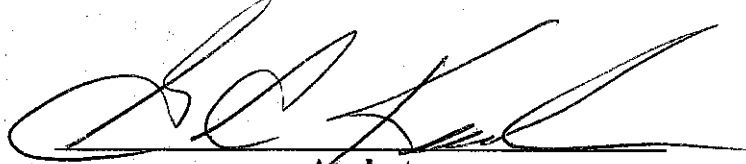
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:37am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:37am |
| CAL  | Pass   | 10:37am |

Preventive Maintenance  
Status: Pass

  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Alamance Co. Instrument Location Burlington P.D.  
Instrument Serial No. 0089011 267 W. Front St  
Burlington, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

ALAMANCE COUNTY BURLINGTON PD 000

Serial Number: 008907

Test Date: 01/06/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

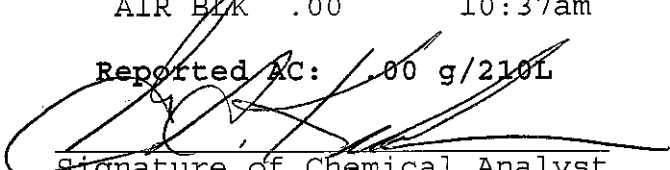
Test Type: Breath Test

Lot Number: AG320602

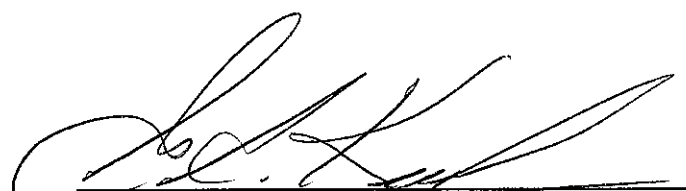
Exp Date: 07/25/2015

| Test            | g/210L     | Time           |
|-----------------|------------|----------------|
| DIAG            | Pass       | 10:30am        |
| AIR BLK         | .00        | 10:31am        |
| ACCY CHK        | .08        | 10:32am        |
| AIR BLK         | .00        | 10:33am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>10:34am</b> |
| AIR BLK         | .00        | 10:35am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>10:36am</b> |
| AIR BLK         | .00        | 10:37am        |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures**  
**Forensic Tests for Alcohol Branch**  
**Department of Health and Human Services**  
**Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

ALAMANCE COUNTY BURLINGTON PD 000

Serial Number: 008907      Test Record Number: 662  
Test Date: 01/06/2015      Test Time: 10:45am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:46am |
| FLO  | Pass   | 10:46am |
| FC   | Pass   | 10:46am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:46am |
| SRC  | Pass   | 10:46am |
| DET  | Pass   | 10:46am |
| BAR  | Pass   | 10:46am |
| BT   | Pass   | 10:46am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:47am |

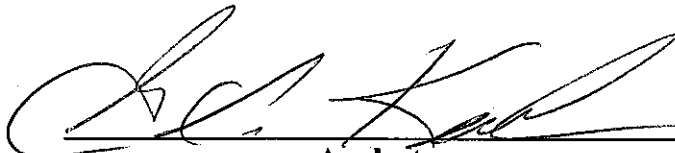
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:47am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:47am |
| CAL  | Pass   | 10:47am |

Preventive Maintenance  
Status: Pass

  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County ALAMANCE


Instrument Location ALAMANCE Co. Jail

Instrument Serial No. 008913 109 S Maple St.  
Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of JANUARY, 2013 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

654

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**-Intox EC/IR-II: Subject Test**

ALAMANCE COUNTY ALAMANCE CO. JAIL 000

Serial Number: 008913

Test Date: 01/06/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

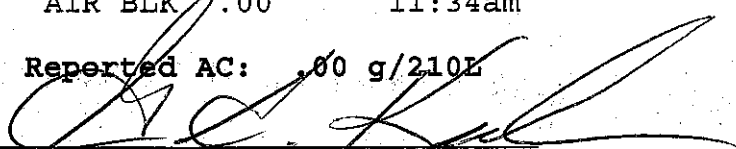
Test Type: Breath Test

Lot Number: AG320602

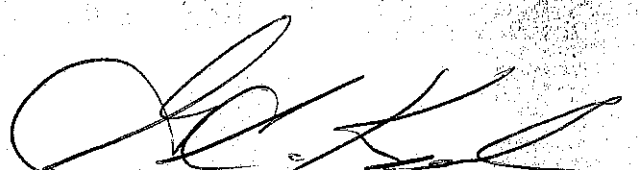
Exp Date: 07/25/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:26am |
| AIR BLK  | .00    | 11:27am |
| ACCY CHK | .08    | 11:28am |
| AIR BLK  | .00    | 11:29am |
| SUB TEST | .00    | 11:30am |
| AIR BLK  | .00    | 11:31am |
| SUB TEST | .00    | 11:33am |
| AIR BLK  | .00    | 11:34am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007



**Intox EC/IR-II: Preventive Maintenance**

**ALAMANCE COUNTY ALAMANCE CO. JAIL 000**

Serial Number: 008913      Test Record Number: 2065  
Test Date: 01/06/2015      Test Time: 11:35am EST

System Check: Passed

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:36am |
| FLO  | Pass   | 11:36am |
| FC   | Pass   | 11:36am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:36am |
| SRC  | Pass   | 11:36am |
| DET  | Pass   | 11:36am |
| BAR  | Pass   | 11:36am |
| BT   | Pass   | 11:36am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:36am |

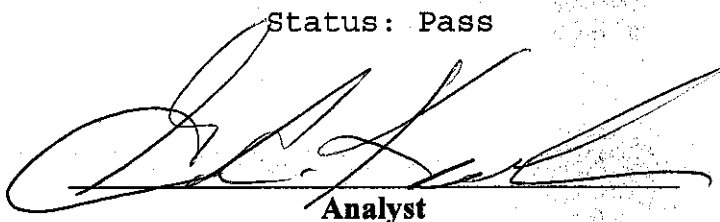
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:37am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:37am |
| CAL  | Pass   | 11:37am |

Preventive Maintenance  
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Alamance Instrument Location Alamance Co. Jail  
Instrument Serial No 008853 109 Maple St  
Graham, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 6 day of JANUARY, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

ALAMANCE COUNTY ALAMANCE CO JAIL 000

Serial Number: 008853

Test Date: 01/06/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: NC

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG322601

Exp Date: 08/14/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:25am |
| AIR BLK  | .00    | 11:26am |
| ACCY CHK | .08    | 11:27am |
| AIR BLK  | .00    | 11:28am |
| SUB TEST | .00    | 11:29am |
| AIR BLK  | .00    | 11:30am |
| SUB TEST | .00    | 11:31am |
| AIR BLK  | .00    | 11:32am |

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

**Intox EC/IR-II: Preventive Maintenance**

**ALAMANCE COUNTY ALAMANCE CO. JAIL 000**

Serial Number: 008853      Test Record Number: 1578  
Test Date: 01/06/2015      Test Time: 11:34am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:35am |
| FLO  | Pass   | 11:35am |
| FC   | Pass   | 11:35am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FCI  | Pass   | 11:35am |
| SRC  | Pass   | 11:35am |
| DET  | Pass   | 11:35am |
| BAR  | Pass   | 11:35am |
| BT   | Pass   | 11:35am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:36am |

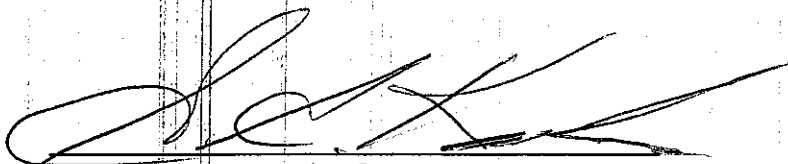
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:36am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:36am |
| CAL  | Pass   | 11:36am |

Preventive Maintenance  
Status: Pass



**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wake

Instrument Location BAT Mobile Unit #7


Instrument Serial No. 008778

Receipt

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16<sup>th</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

636  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: 008778      Test Record Number: 1305  
Test Date: 01/16/2015      Test Time: 11:55pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:56pm |
| FLO  | Pass   | 11:56pm |
| FC   | Pass   | 11:56pm |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:56pm |
| SRC  | Pass   | 11:56pm |
| DET  | Pass   | 11:56pm |
| BAR  | Pass   | 11:56pm |
| BT   | Pass   | 11:56pm |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:57pm |


**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:57pm |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:57pm |
| CAL  | Pass   | 11:57pm |

Preventive Maintenance  
Status: Pass

  
Analyst

Intox EC/IR-II: Subject Test

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: 008778

Test Date: 01/16/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 9372E

Effective:

09/01/2013-09/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test


Lot Number: AG425303

Exp Date: 09/10/2016

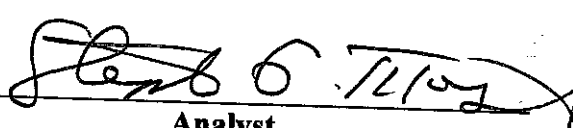
Test g/210L Time

|          |      |         |
|----------|------|---------|
| DIAG     | Pass | 11:47pm |
| AIR BLK  | .00  | 11:48pm |
| ACCY CHK | .08  | 11:48pm |
| AIR BLK  | .00  | 11:49pm |
| SUB TEST | .00  | 11:50pm |
| AIR BLK  | .00  | 11:51pm |
| SUB TEST | .00  | 11:53pm |
| AIR BLK  | .00  | 11:54pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County Wake Instrument Location BAT Mobile Unit #7  
Instrument Serial No. 008377 Ralston

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16<sup>th</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] Signature of Certifying Official 636 Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.



**Intox EC/IR-II: Subject Test**

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: 008577

Test Date: 01/16/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 9372E

Effective:

09/01/2013-09/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG305202

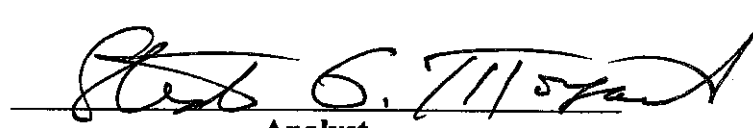
Exp Date: 02/21/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:23pm |
| AIR BLK  | .00    | 10:24pm |
| ACCY CHK | .07    | 10:25pm |
| AIR BLK  | .00    | 10:26pm |
| SUB TEST | .00    | 10:28pm |
| AIR BLK  | .00    | 10:29pm |
| SUB TEST | .00    | 10:30pm |
| AIR BLK  | .00    | 10:31pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County WAKE


Instrument Location RATMOBILE UNIT #7

Instrument Serial No. 008612 RALPH

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16<sup>TH</sup> day of JANUARY, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

1636  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

**WAKE COUNTY BAT MOBILE UNIT 7 910**

Serial Number: 008612      Test Record Number: 1596  
Test Date: 01/16/2015      Test Time: 10:31pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:31pm |
| FLO  | Pass   | 10:31pm |
| FC   | Pass   | 10:31pm |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:32pm |
| SRC  | Pass   | 10:32pm |
| DET  | Pass   | 10:32pm |
| BAR  | Pass   | 10:32pm |
| BT   | Pass   | 10:32pm |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:32pm |

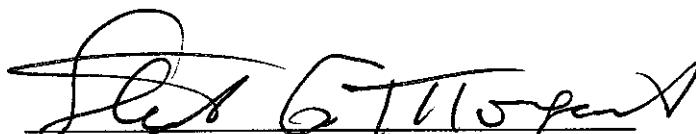
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:32pm |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:32pm |
| CAL  | Pass   | 10:32pm |

Preventive Maintenance  
Status: *Pass*

  
Analyst

**Intox EC/IR-II: Subject Test**

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: 008612  
Test Date: 01/16/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 9372E

Effective:

09/01/2013-09/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG425303

Exp Date: 09/10/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:21pm |
| AIR BLK  | .00    | 10:22pm |
| ACCY CHK | .07    | 10:23pm |
| AIR BLK  | .00    | 10:24pm |
| SUB TEST | .00    | 10:24pm |
| AIR BLK  | .00    | 10:25pm |
| SUB TEST | .00    | 10:27pm |
| AIR BLK  | .00    | 10:28pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County Wake

Instrument Location BAT MOBILE UNIT #7


Instrument Serial No. 008760

TRALEGH

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16<sup>th</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

656  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Preventive Maintenance**

**WAKE COUNTY BAT MOBILE UNIT 7 910**

Serial Number: 008760      Test Record Number: 688  
Test Date: 01/16/2015      Test Time: 10:10pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:10pm |
| FLO  | Pass   | 10:10pm |
| FC   | Pass   | 10:10pm |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:10pm |
| SRC  | Pass   | 10:10pm |
| DET  | Pass   | 10:10pm |
| BAR  | Pass   | 10:10pm |
| BT   | Pass   | 10:10pm |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:11pm |


**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:11pm |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:11pm |
| CAL  | Pass   | 10:11pm |

Preventive Maintenance  
Status: *Pass*

  
**Analyst**

**Intox EC/IR-II: Subject Test**

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: 008760

Test Date: 01/16/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 9372E

Effective:

09/01/2013-09/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG305202

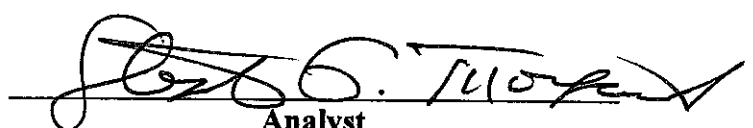
Exp Date: 02/21/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:02pm |
| AIR BLK  | .00    | 10:03pm |
| ACCY CHK | .08    | 10:03pm |
| AIR BLK  | .00    | 10:04pm |
| SUB TEST | .00    | 10:05pm |
| AIR BLK  | .00    | 10:06pm |
| SUB TEST | .00    | 10:07pm |
| AIR BLK  | .00    | 10:08pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wake

Instrument Location BAT MOBILE UNIT #7


Instrument Serial No. DD8972

RALPH

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 16<sup>th</sup> day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]

Signature of Certifying Official

636

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.



**Intox EC/IR-II: Preventive Maintenance**

**WAKE COUNTY BAT MOBILE UNIT 7 910**

Serial Number: 008972      Test Record Number: 38  
Test Date: 01/16/2015      Test Time: 10:08pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:08pm |
| FLO  | Pass   | 10:08pm |
| FC   | Pass   | 10:09pm |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:09pm |
| SRC  | Pass   | 10:09pm |
| DET  | Pass   | 10:09pm |
| BAR  | Pass   | 10:09pm |
| BT   | Pass   | 10:09pm |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:09pm |

**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:09pm |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:09pm |
| CAL  | Pass   | 10:09pm |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

**Intox EC/IR-II: Subject Test**

WAKE COUNTY BAT MOBILE UNIT 7 910

Serial Number: 008972

Test Date: 01/16/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: MORGART, STEPHEN G

Permit Number: 9372E

Effective:

09/01/2013-09/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG425303

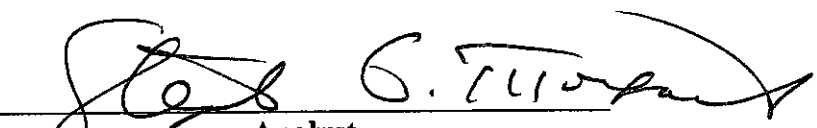
Exp Date: 10/10/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:00pm |
| AIR BLK  | .00    | 10:01pm |
| ACCY CHK | .08    | 10:01pm |
| AIR BLK  | .00    | 10:02pm |
| SUB TEST | .00    | 10:03pm |
| AIR BLK  | .00    | 10:04pm |
| SUB TEST | .00    | 10:06pm |
| AIR BLK  | .00    | 10:07pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County CARTERET Instrument Location BAT MOBILE UNIT 3  
Instrument Serial No. 008647 MOREHEAD CITY, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 10 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Celina R. B...  
Signature of Certifying Official

648  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**CARTERET COUNTY BAT MOBILE UNIT 3 150**

Serial Number: 008647

Test Date: 01/10/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BARNES, ALVIN R

Permit Number: 15671E

Effective:

09/01/2013-09/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG414801


Exp Date: 05/28/2016

| Test            | g/210L     | Time           |
|-----------------|------------|----------------|
| DIAG            | Pass       | 11:13pm        |
| AIR BLK         | .00        | 11:14pm        |
| ACCY CHK        | .08        | 11:15pm        |
| AIR BLK         | .00        | 11:16pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>11:17pm</b> |
| AIR BLK         | .00        | 11:18pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>11:19pm</b> |
| AIR BLK         | .00        | 11:20pm        |

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**CARTERET COUNTY BAT MOBILE UNIT 3 150**

Serial Number: 008647      Test Record Number: 2053  
Test Date: 01/10/2015      Test Time: 11:21pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:21pm |
| FLO  | Pass   | 11:21pm |
| FC   | Pass   | 11:21pm |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:21pm |
| SRC  | Pass   | 11:21pm |
| DET  | Pass   | 11:21pm |
| BAR  | Pass   | 11:21pm |
| BT   | Pass   | 11:21pm |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:22pm |


**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:22pm |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:22pm |
| CAL  | Pass   | 11:22pm |

Preventive Maintenance  
Status: Pass

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**


County Wake Co. Instrument Location Wake Co. Detention Center

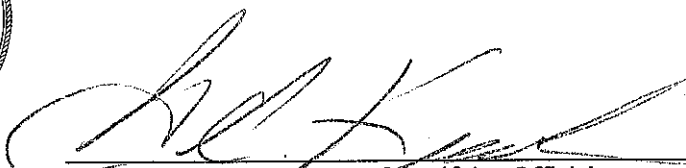
Instrument Serial No. 008826 3301 Hammond Rd Raleigh, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 30 day of JANUARY, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



  
Signature of Certifying Official

634  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008826

Test Date: 01/30/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG434201

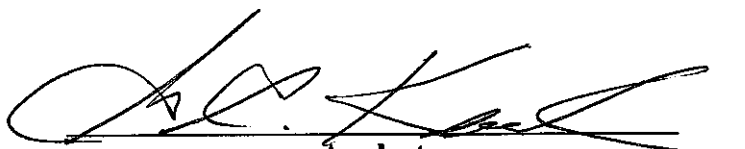
Exp Date: 12/08/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 12:22pm |
| AIR BLK  | .00    | 12:23pm |
| ACCY CHK | .08    | 12:23pm |
| AIR BLK  | .00    | 12:25pm |
| SUB TEST | .00    | 12:26pm |
| AIR BLK  | .00    | 12:27pm |
| SUB TEST | .00    | 12:28pm |
| AIR BLK  | .00    | 12:29pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

# Intox EC/IR-II: Preventive Maintenance

WAKE COUNTY DETENTION CENTER 910

Serial Number: 008826 Test Record Number: 7858

Test Date: 01/30/2015 Test Time: 12:30pm EST

System Check: Passed

## Baseline Tests

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 12:30pm |
| FLO  | Pass   | 12:30pm |
| FC   | Pass   | 12:30pm |

## Temperature Tests

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 12:31pm |
| SRC  | Pass   | 12:31pm |
| DET  | Pass   | 12:31pm |
| BAR  | Pass   | 12:31pm |
| BT   | Pass   | 12:31pm |

## Blank Tests

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 12:31pm |

## Printer Tests

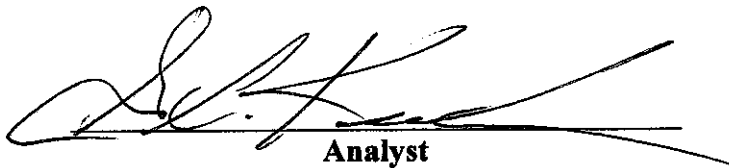
| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 12:31pm |

## CRC Tests

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 12:31pm |
| CAL  | Pass   | 12:31pm |

Preventive Maintenance

Status: Pass



Analyst



DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County

Johnston

Instrument Location

Johnston Co. Jail

Instrument Serial No.


008846

Smithfield, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27<sup>th</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Dale Farley  
Signature of Certifying Official

655  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

JOHNSTON COUNTY JOHNSTON CO. JAIL 500

Serial Number: 008846

Test Date: 01/27/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2014-11/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

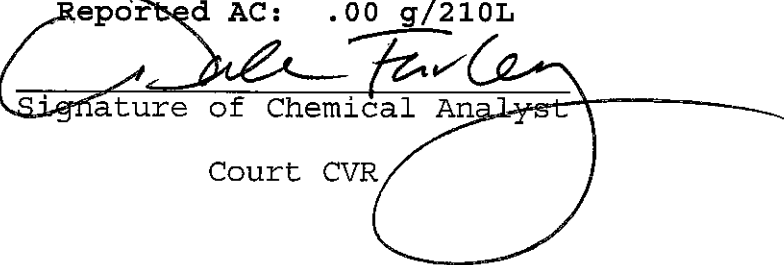
Test Type: Breath Test

Lot Number: AG411202

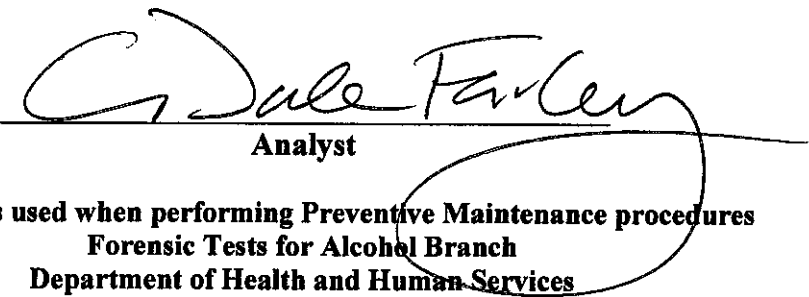
Exp Date: 04/22/2016

| Test            | g/210L     | Time           |
|-----------------|------------|----------------|
| DIAG            | Pass       | 10:37am        |
| AIR BLK         | .00        | 10:38am        |
| ACCY CHK        | .08        | 10:39am        |
| AIR BLK         | .00        | 10:40am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>10:42am</b> |
| AIR BLK         | .00        | 10:43am        |
| <b>SUB TEST</b> | <b>.00</b> | <b>10:45am</b> |
| AIR BLK         | .00        | 10:46am        |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

# Intox EC/IR-II: Preventive Maintenance

JOHNSTON COUNTY JOHNSTON CO. JAIL 500  
Serial Number: 008846      Test Record Number: 3574  
Test Date: 01/27/2015      Test Time: 10:53am EST  
System Check: Passed

## Baseline Tests

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:54am |
| FLO  | Pass   | 10:54am |
| FC   | Pass   | 10:54am |

## Temperature Tests

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:54am |
| SRC  | Pass   | 10:54am |
| DET  | Pass   | 10:54am |
| BAR  | Pass   | 10:54am |
| BT   | Pass   | 10:54am |

## Blank Tests

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:55am |

## Printer Tests

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:55am |

## CRC Tests

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:55am |
| CAL  | Pass   | 10:55am |

Preventive Maintenance  
Status: Pass

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Lee Instrument Location Lee County Jail  
Instrument Serial No. 008645 Sanford, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26<sup>th</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature] 655  
Signature of Certifying Official Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

LEE COUNTY LEE CO. LEC. 520

Serial Number: 008645

Test Date: 01/26/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2014-11/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

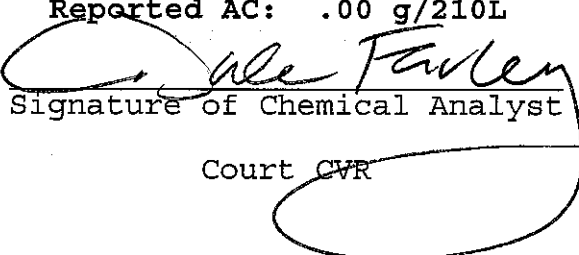
Test Type: Breath Test

Lot Number: AG414801

Exp Date: 05/28/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 9:27am |
| AIR BLK  | .00    | 9:27am |
| ACCY CHK | .08    | 9:28am |
| AIR BLK  | .00    | 9:29am |
| SUB TEST | .00    | 9:30am |
| AIR BLK  | .00    | 9:31am |
| SUB TEST | .00    | 9:32am |
| AIR BLK  | .00    | 9:33am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

# Intox EC/IR-II: Preventive Maintenance

LEE COUNTY LEE CO. LEC. 520

Serial Number: 008645      Test Record Number: 1454  
Test Date: 01/26/2015      Test Time: 9:35am EST

System Check: *Passed*

## Baseline Tests

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 9:35am |
| FLO  | Pass   | 9:35am |
| FC   | Pass   | 9:35am |

## Temperature Tests

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 9:35am |
| SRC  | Pass   | 9:35am |
| DET  | Pass   | 9:35am |
| BAR  | Pass   | 9:35am |
| BT   | Pass   | 9:35am |

## Blank Tests

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 9:36am |


## Printer Tests

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 9:36am |

## CRC Tests

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 9:36am |
| CAL  | Pass   | 9:36am |

Preventive Maintenance  
Status: Pass

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Lee Instrument Location Sanford Police Dept.  
Instrument Serial No. 008867 Sanford, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22<sup>nd</sup> day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

655  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

LEE COUNTY SANFORD POLICE DEPT 520

Serial Number: 008867

Test Date: 01/22/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2014-11/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

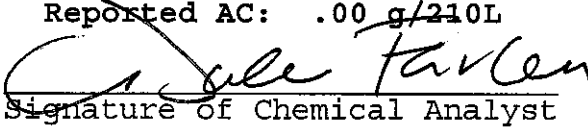
Test Type: Breath Test

Lot Number: AG320602

Exp Date: 07/25/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 5:13pm |
| AIR BLK  | .00    | 5:15pm |
| ACCY CHK | .07    | 5:15pm |
| AIR BLK  | .00    | 5:16pm |
| SUB TEST | .00    | 5:17pm |
| AIR BLK  | .00    | 5:18pm |
| SUB TEST | .00    | 5:19pm |
| AIR BLK  | .00    | 5:20pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007



**Intox EC/IR-II: Preventive Maintenance**

**LEE COUNTY SANFORD POLICE DEPT 520**

Serial Number: 008867      Test Record Number: 836  
Test Date: 01/22/2015      Test Time: 5:21pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 5:22pm |
| FLO  | Pass   | 5:22pm |
| FC   | Pass   | 5:22pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 5:22pm |
| SRC  | Pass   | 5:22pm |
| DET  | Pass   | 5:22pm |
| BAR  | Pass   | 5:22pm |
| BT   | Pass   | 5:22pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 5:23pm |

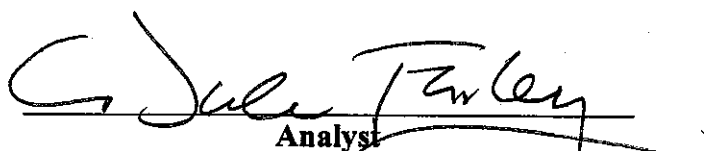
**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 5:23pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 5:23pm |
| CAL  | Pass   | 5:23pm |

Preventive Maintenance  
Status: Pass

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County Montgomery Instrument Location Montgomery Co. Jail  
Instrument Serial No. 008657 Tray N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12<sup>th</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

655  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

MONTGOMERY COUNTY MONTGOMERY CO. JAIL  
610

Serial Number: 008657

Test Date: 01/12/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: FARLEY, CYNTHIA D

Permit Number: 24123E

Effective:

11/01/2014-11/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

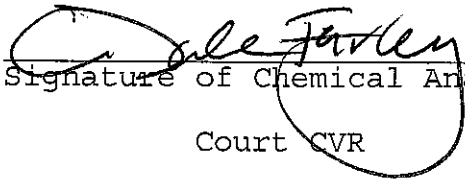
Test Type: Breath Test

Lot Number: AG414801

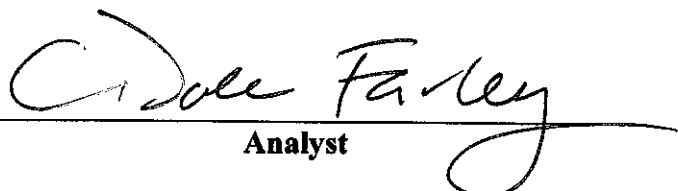
Exp Date: 05/28/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 8:16pm |
| AIR BLK  | .00    | 8:17pm |
| ACCY CHK | .07    | 8:18pm |
| AIR BLK  | .00    | 8:19pm |
| SUB TEST | .00    | 8:19pm |
| AIR BLK  | .00    | 8:20pm |
| SUB TEST | .00    | 8:22pm |
| AIR BLK  | .00    | 8:23pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

**Intox EC/IR-II: Preventive Maintenance**

**MONTGOMERY COUNTY MONTGOMERY CO. JAIL 610**

Serial Number: 008657      Test Record Number: 1009  
Test Date: 01/12/2015      Test Time: 8:24pm EST

System Check: Passed

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 8:24pm |
| FLO  | Pass   | 8:24pm |
| FC   | Pass   | 8:24pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 8:25pm |
| SRC  | Pass   | 8:25pm |
| DET  | Pass   | 8:25pm |
| BAR  | Pass   | 8:25pm |
| BT   | Pass   | 8:25pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 8:25pm |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 8:25pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 8:25pm |
| CAL  | Pass   | 8:25pm |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Halifax Instrument Location Roanoke Rapids P.D.

Instrument Serial No. 008635 1040 Roanoke Ave  
Roanoke Rapids, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

HALIFAX CO ROANOKE RAPIDS PD 410

Serial Number: 008635

Test Date: 01/20/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

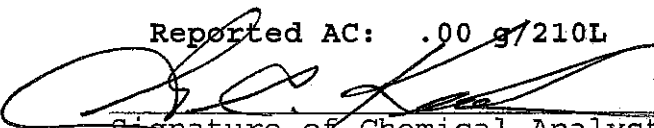
Test Type: Breath Test

Lot Number: AG411202

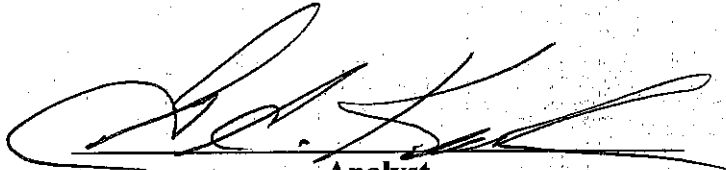
Exp Date: 04/22/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 1:11pm |
| AIR BLK  | .00    | 1:12pm |
| ACCY CHK | .08    | 1:12pm |
| AIR BLK  | .00    | 1:14pm |
| SUB TEST | .00    | 1:15pm |
| AIR BLK  | .00    | 1:16pm |
| SUB TEST | .00    | 1:17pm |
| AIR BLK  | .00    | 1:18pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures**

**Forensic Tests for Alcohol Branch**

**Department of Health and Human Services**

**Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

**HALIFAX CO ROANOKE RAPIDS PD 410**

Serial Number: 008635      Test Record Number: 1378  
Test Date: 01/20/2015      Test Time: 1:21pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 1:21pm |
| FLO  | Pass   | 1:21pm |
| FC   | Pass   | 1:21pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 1:21pm |
| SRC  | Pass   | 1:21pm |
| DET  | Pass   | 1:21pm |
| BAR  | Pass   | 1:21pm |
| BT   | Pass   | 1:21pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 1:22pm |

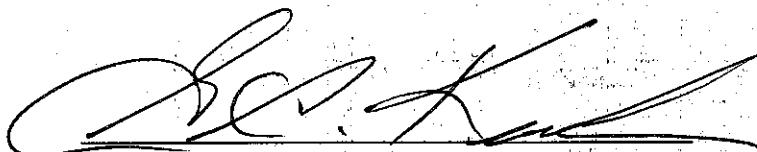
**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 1:22pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 1:22pm |
| CAL  | Pass   | 1:22pm |

Preventive Maintenance  
Status: *Pass*

  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County Halifax Instrument Location Roanoke Rapids P.D.

Instrument Serial No. 008656 1040 Roanoke Ave  
Roanoke Rapids, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.



**Intox EC/IR-II: Subject Test**

HALIFAX CO. ROANOKE RAPIDS PD 410

Serial Number: 008656

Test Date: 01/20/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

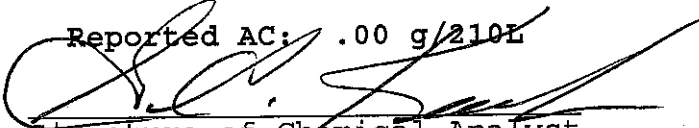
Test Type: Breath Test

Lot Number: AG411202

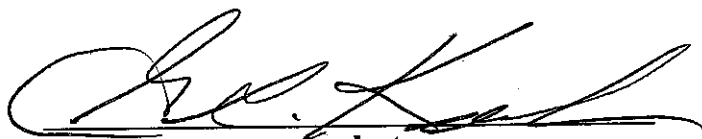
Exp Date: 04/22/2016

| Test            | g/210L     | Time          |
|-----------------|------------|---------------|
| DIAG            | Pass       | 1:13pm        |
| AIR BLK         | .00        | 1:14pm        |
| ACCY CHK        | .07        | 1:15pm        |
| AIR BLK         | .00        | 1:16pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>1:16pm</b> |
| AIR BLK         | .00        | 1:18pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>1:19pm</b> |
| AIR BLK         | .00        | 1:20pm        |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures**

**Forensic Tests for Alcohol Branch**

**Department of Health and Human Services**

**Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

**HALIFAX CO. ROANOKE RAPIDS PD 410**

Serial Number: 008656      Test Record Number: 507  
Test Date: 01/20/2015      Test Time: 1:22pm EST

**System Check: Passed**

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 1:22pm |
| FLO  | Pass   | 1:22pm |
| FC   | Pass   | 1:22pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 1:22pm |
| SRC  | Pass   | 1:22pm |
| DET  | Pass   | 1:22pm |
| BAR  | Pass   | 1:22pm |
| BT   | Pass   | 1:22pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 1:23pm |

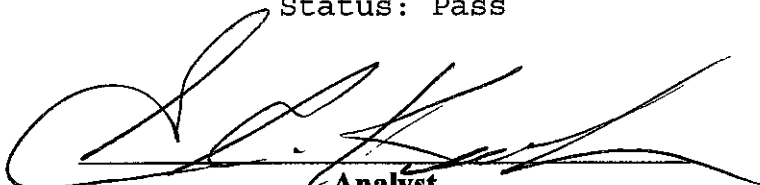
**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 1:23pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 1:23pm |
| CAL  | Pass   | 1:23pm |

**Preventive Maintenance**  
Status: Pass

  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Northampton Instrument Location Northampton Co. Sheriff Dept  
Instrument Serial No. 008607 105 W Jefferson St Jackson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**NORTHAMPTON COUNTY SHERIFFS DEPARTMENT**  
650

Serial Number: 008607  
Test Date: 01/20/2015

Citation Number: M0000000-0  
Subject's Name:  
PREVENTIVE, MAINTENANCE  
Subject's Date of Birth: 11/11/1911  
Subject's Sex: Male  
Driver's License State: XX  
Driver's License Number: NONE

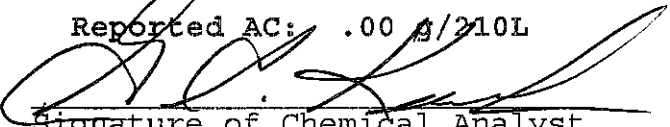
Analyst's Name: KEESLER, GRAYHAM C  
Permit Number: 7682E  
Effective:  
02/01/2014-02/01/2016

Officer's Name: NONE, NONE  
Type of Agency: FTA  
Agency: DHHS  
Test Type: Breath Test

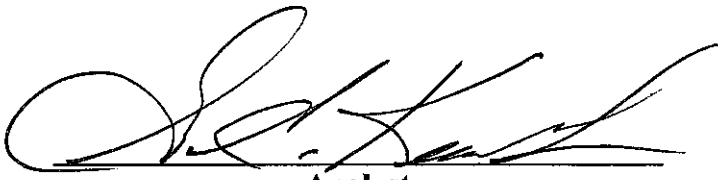
Lot Number: AG411202  
Exp Date: 04/22/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:59am |
| AIR BLK  | .00    | 12:00pm |
| ACCY CHK | .07    | 12:00pm |
| AIR BLK  | .00    | 12:01pm |
| SUB TEST | .00    | 12:02pm |
| AIR BLK  | .00    | 12:03pm |
| SUB TEST | .00    | 12:05pm |
| AIR BLK  | .00    | 12:05pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**NORTHAMPTON COUNTY SHERIFFS DEPARTMENT 650**

Serial Number: 008607      Test Record Number: 768  
Test Date: 01/20/2015      Test Time: 12:07pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 12:07pm |
| FLO  | Pass   | 12:07pm |
| FC   | Pass   | 12:07pm |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 12:07pm |
| SRC  | Pass   | 12:07pm |
| DET  | Pass   | 12:07pm |
| BAR  | Pass   | 12:07pm |
| BT   | Pass   | 12:07pm |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 12:08pm |

**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 12:08pm |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 12:08pm |
| CAL  | Pass   | 12:08pm |

Preventive Maintenance  
Status: Pass

  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Northampton Instrument Location Northampton Co. Sheriff's Dept.  
Instrument Serial No. 008688 105 W. Jefferson St. Jackson, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of JANUARY, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**NORTHAMPTON COUNTY SHERIFFS DEPARTMENT**  
650

Serial Number: 008688  
Test Date: 01/20/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

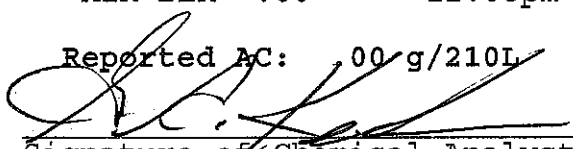
Lot Number: AG425303

Exp Date: 09/10/2016

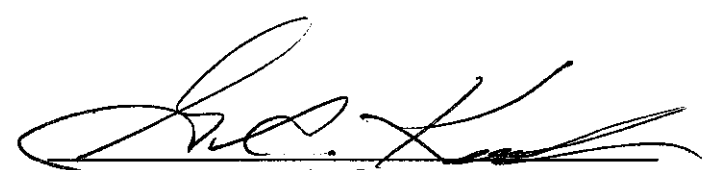
Test        g/210L        Time

|          |      |         |
|----------|------|---------|
| DIAG     | Pass | 12:01pm |
| AIR BLK  | .00  | 12:02pm |
| ACCY CHK | .07  | 12:03pm |
| AIR BLK  | .00  | 12:04pm |
| SUB TEST | .00  | 12:05pm |
| AIR BLK  | .00  | 12:06pm |
| SUB TEST | .00  | 12:08pm |
| AIR BLK  | .00  | 12:08pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures**  
**Forensic Tests for Alcohol Branch**  
**Department of Health and Human Services**  
**Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

**NORTHAMPTON COUNTY SHERIFFS DEPARTMENT 650**

Serial Number: 008688      Test Record Number: 699  
Test Date: 01/20/2015      Test Time: 12:10pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 12:10pm |
| FLO  | Pass   | 12:10pm |
| FC   | Pass   | 12:10pm |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 12:10pm |
| SRC  | Pass   | 12:10pm |
| DET  | Pass   | 12:10pm |
| BAR  | Pass   | 12:10pm |
| BT   | Pass   | 12:10pm |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 12:11pm |

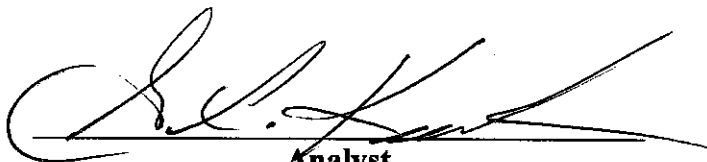
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 12:11pm |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 12:11pm |
| CAL  | Pass   | 12:11pm |

Preventive Maintenance  
Status: Pass

  
**Analyst**



DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County Halifax Instrument Location Halifax Co. S.O.  
Instrument Serial No. 008695 355 FERRELL LANE  
Halifax, NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

HALIFAX CO. HALIFAX CO. SD 410

Serial Number: 008695

Test Date: 01/20/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, GRAYHAM C

Permit Number: 7682E

Effective:

02/01/2014-02/01/2016

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG411202

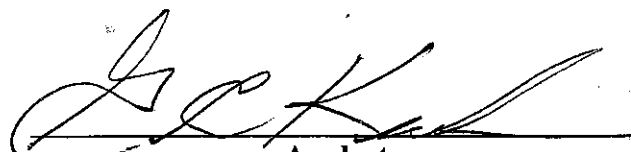
Exp Date: 04/22/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:46am |
| AIR BLK  | .00    | 10:47am |
| ACCY CHK | .08    | 10:48am |
| AIR BLK  | .00    | 10:49am |
| SUB TEST | .00    | 10:49am |
| AIR BLK  | .00    | 10:50am |
| SUB TEST | .00    | 10:52am |
| AIR BLK  | .00    | 10:53am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

# Intox EC/IR-II: Preventive Maintenance

HALIFAX CO. HALIFAX CO. SD 410

Serial Number: 008695 Test Record Number: 1739  
Test Date: 01/20/2015 Test Time: 10:56am EST

System Check: Passed

## Baseline Tests

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 10:57am |
| FLO  | Pass   | 10:57am |
| FC   | Pass   | 10:57am |

## Temperature Tests

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 10:57am |
| SRC  | Pass   | 10:57am |
| DET  | Pass   | 10:57am |
| BAR  | Pass   | 10:57am |
| BT   | Pass   | 10:57am |

## Blank Tests

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 10:57am |

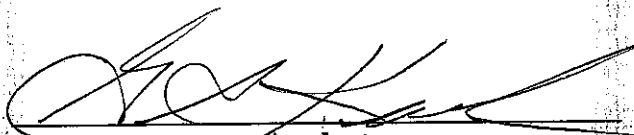
## Printer Tests

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 10:58am |

## CRC Tests

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 10:58am |
| CAL  | Pass   | 10:58am |

Preventive Maintenance  
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Dare Instrument Location Kill Devil Hills P.D.  
Instrument Serial No. 008844 102 Town Hall Dr., Kill Devil Hills,  
N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23<sup>rd</sup> day of JANUARY, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Lois A. Hester  
Signature of Certifying Official

647  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**DARE COUNTY KILL DEVIL HILLS PD 270**

Serial Number: 008844

Test Date: 01/23/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A

Permit Number: 11646E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG335201


Exp Date: 12/18/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 2:36pm |
| AIR BLK  | .00    | 2:37pm |
| ACCY CHK | .08    | 2:37pm |
| AIR BLK  | .00    | 2:39pm |
| SUB TEST | .00    | 2:39pm |
| AIR BLK  | .00    | 2:40pm |
| SUB TEST | .00    | 2:42pm |
| AIR BLK  | .00    | 2:43pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**DARE COUNTY KILL DEVIL HILLS PD 270**

Serial Number: 008844      Test Record Number: 1553  
Test Date: 01/23/2015      Test Time: 2:44pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 2:45pm |
| FLO  | Pass   | 2:45pm |
| FC   | Pass   | 2:45pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 2:45pm |
| SRC  | Pass   | 2:45pm |
| DET  | Pass   | 2:45pm |
| BAR  | Pass   | 2:45pm |
| BT   | Pass   | 2:45pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 2:46pm |

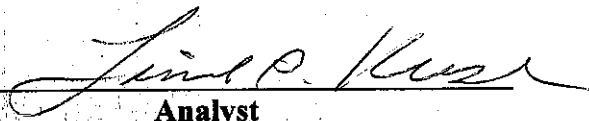
**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 2:46pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 2:46pm |
| CAL  | Pass   | 2:46pm |

Preventive Maintenance  
Status: *Pass*

  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Currituck Instrument Location Currituck Co. S.O. - Corolla  
Instrument Serial No. 008949 1123 Ocean Trail, Corolla, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23<sup>rd</sup> day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linda A. Kuse  
Signature of Certifying Official

047  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**CURRITUCK COUNTY SO-COROLLA 260**

Serial Number: 008949

Test Date: 01/23/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A

Permit Number: 11646E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG315701


Exp Date: 06/06/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 1:07pm |
| AIR BLK  | .00    | 1:08pm |
| ACCY CHK | .08    | 1:09pm |
| AIR BLK  | .00    | 1:10pm |
| SUB TEST | .00    | 1:10pm |
| AIR BLK  | .00    | 1:11pm |
| SUB TEST | .00    | 1:13pm |
| AIR BLK  | .00    | 1:14pm |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst



**Intox EC/IR-II: Preventive Maintenance**

*CURRITUCK COUNTY SO-COROLLA 260*

Serial Number: 008949      Test Record Number: 356  
Test Date: 01/23/2015      Test Time: 1:15pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 1:15pm |
| FLO  | Pass   | 1:15pm |
| FC   | Pass   | 1:15pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 1:15pm |
| SRC  | Pass   | 1:15pm |
| DET  | Pass   | 1:15pm |
| BAR  | Pass   | 1:15pm |
| BT   | Pass   | 1:15pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 1:16pm |


**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 1:16pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 1:16pm |
| CAL  | Pass   | 1:16pm |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Edgecombe Instrument Location Edgecombe Co. Magistrate's  
Instrument Serial No. 004663 office, 300 S. Anaconda Rd., Tarboro  
NC.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22nd day of JANUARY, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



James S. Kessel  
Signature of Certifying Official

647  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR  
320

Serial Number: 008663

Test Date: 01/22/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A

Permit Number: 11646E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG411202


Exp Date: 04/22/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 4:09pm |
| AIR BLK  | .00    | 4:10pm |
| ACCY CHK | .07    | 4:11pm |
| AIR BLK  | .00    | 4:12pm |
| SUB TEST | .00    | 4:12pm |
| AIR BLK  | .00    | 4:13pm |
| SUB TEST | .00    | 4:15pm |
| AIR BLK  | .00    | 4:16pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320**

Serial Number: 008663      Test Record Number: 2279  
Test Date: 01/22/2015      Test Time: 4:17pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 4:18pm |
| FLO  | Pass   | 4:18pm |
| FC   | Pass   | 4:18pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 4:18pm |
| SRC  | Pass   | 4:18pm |
| DET  | Pass   | 4:18pm |
| BAR  | Pass   | 4:18pm |
| BT   | Pass   | 4:18pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 4:19pm |


**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 4:19pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 4:19pm |
| CAL  | Pass   | 4:19pm |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County Edgecombe Instrument Location Edgecombe Co. Magistrate's  
Instrument Serial No. 004603 Office, 300 S. Apacanda Rd, Tarboro,  
N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22<sup>nd</sup> day of JANUARY, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



James Russell  
Signature of Certifying Official

647  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

EDGECOMBE COUNTY EDGECOMBE CO MAGISTR  
320

Serial Number: 008603

Test Date: 01/22/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A

Permit Number: 11646E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG320602


Exp Date: 07/25/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 4:10pm |
| AIR BLK  | .00    | 4:11pm |
| ACCY CHK | .08    | 4:12pm |
| AIR BLK  | .00    | 4:12pm |
| SUB TEST | .00    | 4:13pm |
| AIR BLK  | .00    | 4:14pm |
| SUB TEST | .00    | 4:16pm |
| AIR BLK  | .00    | 4:17pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007

**Intox EC/IR-II: Preventive Maintenance**

**EDGECOMBE COUNTY EDGECOMBE CO MAGISTR 320**

Serial Number: 008603      Test Record Number: 1433  
Test Date: 01/22/2015      Test Time: 4:19pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 4:19pm |
| FLO  | Pass   | 4:19pm |
| FC   | Pass   | 4:19pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 4:19pm |
| SRC  | Pass   | 4:19pm |
| DET  | Pass   | 4:19pm |
| BAR  | Pass   | 4:19pm |
| BT   | Pass   | 4:19pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 4:20pm |


**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 4:20pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 4:20pm |
| CAL  | Pass   | 4:20pm |

Preventive Maintenance  
Status: Pass



**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Currituck Instrument Location Currituck Co. S.O.  
Instrument Serial No. 008947 407-A Maple Rd., Maple, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22<sup>nd</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



James H. Hester  
Signature of Certifying Official

647  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.



**Intox EC/IR-II: Subject Test**

**CURRITUCK COUNTY CURRITUCK SO-MAPLE**  
**260**

Serial Number: 008947

Test Date: 01/22/2015

Citation Number: M0000000-0

Subject's Name:

**PREVENTIVE, MAINTENANCE**

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: **KEESLER, LINDA A**

Permit Number: 11646E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG315701


Exp Date: 06/06/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 1:41pm |
| AIR BLK  | .00    | 1:42pm |
| ACCY CHK | .08    | 1:43pm |
| AIR BLK  | .00    | 1:44pm |
| SUB TEST | .00    | 1:44pm |
| AIR BLK  | .00    | 1:45pm |
| SUB TEST | .00    | 1:47pm |
| AIR BLK  | .00    | 1:48pm |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

Intox EC/IR-II: Preventive Maintenance

CURRITUCK COUNTY CURRITUCK SO-MAPLE 260

Serial Number: 008947      Test Record Number: 1628  
Test Date: 01/22/2015      Test Time: 1:51pm EST

System Check: *Passed*

Baseline Tests

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 1:51pm |
| FLO  | Pass   | 1:51pm |
| FC   | Pass   | 1:51pm |

Temperature Tests

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 1:51pm |
| SRC  | Pass   | 1:51pm |
| DET  | Pass   | 1:51pm |
| BAR  | Pass   | 1:51pm |
| BT   | Pass   | 1:51pm |

Blank Tests

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 1:52pm |


Printer Tests

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 1:52pm |

CRC Tests

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 1:52pm |
| CAL  | Pass   | 1:52pm |

Preventive Maintenance  
Status: Pass

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Wayne Instrument Location Wayne Co. Detention Ctr.  
Instrument Serial No. DD 8671 207 E. Chestnut St., Goldsboro, N.C.

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 12<sup>th</sup> day of JANUARY, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Linda A. Keese  
Signature of Certifying Official

647  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008671

Test Date: 01/12/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: KEESLER, LINDA A

Permit Number: 11646E

Effective:

08/01/2013-08/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG315701

Exp Date: 06/06/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 12:44pm |
| AIR BLK  | .00    | 12:44pm |
| ACCY CHK | .07    | 12:45pm |
| AIR BLK  | .00    | 12:46pm |
| SUB TEST | .00    | 12:47pm |
| AIR BLK  | .00    | 12:48pm |
| SUB TEST | .00    | 12:49pm |
| AIR BLK  | .00    | 12:50pm |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

**This form is used when performing Preventive Maintenance procedures**

**Forensic Tests for Alcohol Branch**

**Department of Health and Human Services**

**Rev. 12/2007**

Intox EC/IR-II: Preventive Maintenance

WAYNE COUNTY WAYNE CO DETENTION 950

Serial Number: 008671 Test Record Number: 3486  
Test Date: 01/12/2015 Test Time: 12:58pm EST

System Check: Passed

Baseline Tests

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 12:59pm |
| FLO  | Pass   | 12:59pm |
| FC   | Pass   | 12:59pm |

Temperature Tests

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 12:59pm |
| SRC  | Pass   | 12:59pm |
| DET  | Pass   | 12:59pm |
| BAR  | Pass   | 12:59pm |
| BT   | Pass   | 12:59pm |

Blank Tests

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 1:00pm |


Printer Tests

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 1:00pm |

CRC Tests

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 1:00pm |
| CAL  | Pass   | 1:00pm |

Preventive Maintenance  
Status: Pass

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg Instrument Location Bd Mobile Unit 5  
Instrument Serial No. 008706

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

658  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**MECKLENBURG BAT MOBILE UNIT 5 590**

Serial Number: 008706

Test Date: 01/22/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TOWERY, CHAD V

Permit Number: 26632E

Effective:

10/18/2013-10/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

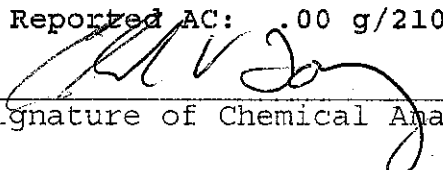
Test Type: Breath Test

Lot Number: AG322601

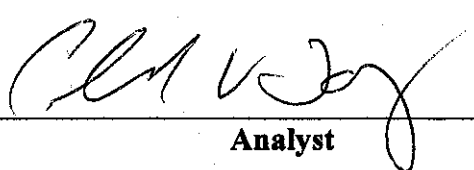
Exp Date: 08/14/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 9:34pm |
| AIR BLK  | .00    | 9:35pm |
| ACCY CHK | .08    | 9:36pm |
| AIR BLK  | .00    | 9:37pm |
| SUB TEST | .00    | 9:37pm |
| AIR BLK  | .00    | 9:38pm |
| SUB TEST | .00    | 9:40pm |
| AIR BLK  | .00    | 9:40pm |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

**MECKLENBURG BAT MOBILE UNIT 5 590**

Serial Number: 008706      Test Record Number: 3354  
Test Date: 01/22/2015      Test Time: 9:42pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 9:43pm |
| FLO  | Pass   | 9:43pm |
| FC   | Pass   | 9:43pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 9:43pm |
| SRC  | Pass   | 9:43pm |
| DET  | Pass   | 9:43pm |
| BAR  | Pass   | 9:43pm |
| BT   | Pass   | 9:43pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 9:43pm |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 9:43pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 9:43pm |
| CAL  | Pass   | 9:43pm |

Preventive Maintenance  
Status: *Pass*

  
\_\_\_\_\_  
**Analyst**



DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg


Instrument Location Bat mobile Unit 5

Instrument Serial No. 008708

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Phil V. Joy

Signature of Certifying Official

658

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**MECKLENBURG BAT MOBILE UNIT 5 590**

Serial Number: 008788

Test Date: 01/22/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TOWERY, CHAD V

Permit Number: 26632E

Effective:

10/18/2013-10/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

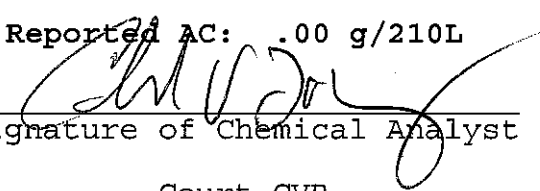
Test Type: Breath Test

Lot Number: AG309101

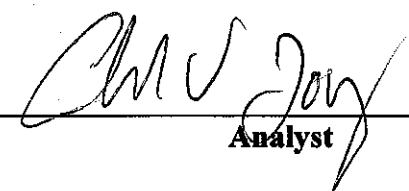
Exp Date: 04/01/2015

| Test            | g/210L     | Time          |
|-----------------|------------|---------------|
| DIAG            | Pass       | 9:33pm        |
| AIR BLK         | .00        | 9:34pm        |
| ACCY CHK        | .07        | 9:35pm        |
| AIR BLK         | .00        | 9:36pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>9:36pm</b> |
| AIR BLK         | .00        | 9:37pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>9:39pm</b> |
| AIR BLK         | .00        | 9:39pm        |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**This form is used when performing Preventive Maintenance procedures**

**Forensic Tests for Alcohol Branch**

**Department of Health and Human Services**

**Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

**MECKLENBURG BAT MOBILE UNIT 5 590**

Serial Number: 008788      Test Record Number: 1139  
Test Date: 01/22/2015      Test Time: 9:40pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 9:41pm |
| FLO  | Pass   | 9:41pm |
| FC   | Pass   | 9:41pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 9:41pm |
| SRC  | Pass   | 9:41pm |
| DET  | Pass   | 9:41pm |
| BAR  | Pass   | 9:41pm |
| BT   | Pass   | 9:41pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 9:42pm |

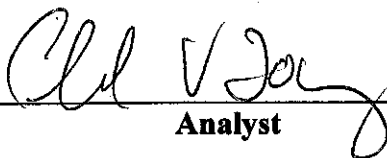
**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 9:42pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 9:42pm |
| CAL  | Pass   | 9:42pm |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Mecklenburg


Instrument Location But mobile Unit 5

Instrument Serial No. 00 8698

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 22 day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Phil V. [Signature]  
Signature of Certifying Official

658

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

MECKLENBURG BAT MOBILE UNIT 5 590

Serial Number: 008698

Test Date: 01/22/2015

Citation Number: M00000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: TOWERY, CHAD V

Permit Number: 26632E

Effective:

10/18/2013-10/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

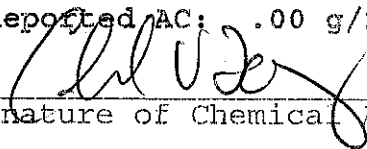
Test Type: Breath Test

Lot Number: AG425303

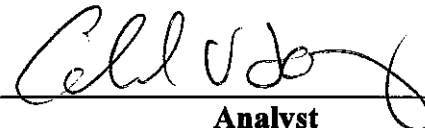
Exp Date: 09/10/2016

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 9:32pm |
| AIR BLK  | .00    | 9:33pm |
| ACCY CHK | .07    | 9:34pm |
| AIR BLK  | .00    | 9:35pm |
| SUB TEST | .00    | 9:35pm |
| AIR BLK  | .00    | 9:36pm |
| SUB TEST | .00    | 9:37pm |
| AIR BLK  | .00    | 9:38pm |

Reported AC: .00 g/210L

  
\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

Intox EC/IR-II: Preventive Maintenance

MECKLENBURG BAT MOBILE UNIT 5 590

Serial Number: 008698      Test Record Number: 1231  
Test Date: 01/22/2015      Test Time: 9:39pm EST

System Check: Passed

Baseline Tests

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 9:39pm |
| FLO  | Pass   | 9:39pm |
| FC   | Pass   | 9:40pm |

Temperature Tests

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 9:40pm |
| SRC  | Pass   | 9:40pm |
| DET  | Pass   | 9:40pm |
| BAR  | Pass   | 9:40pm |
| BT   | Pass   | 9:40pm |

Blank Tests

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 9:40pm |

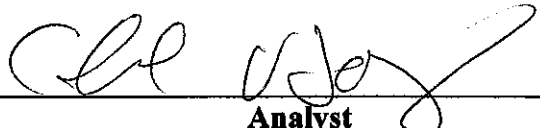
Printer Tests

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 9:40pm |

CRC Tests

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 9:41pm |
| CAL  | Pass   | 9:41pm |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Gaston Instrument Location Gaston County SD  
Instrument Serial No. 008643 425 N. Marietta Street, Gastonia  
704-869-6800

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23rd day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hitt  
Signature of Certifying Official

650  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

GASTON COUNTY GASTON COUNTY SD 350

Serial Number: 008643

Test Date: 01/23/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

10/01/2013-10/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS

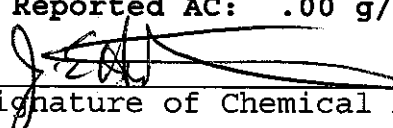
Test Type: Breath Test

Lot Number: AG335201

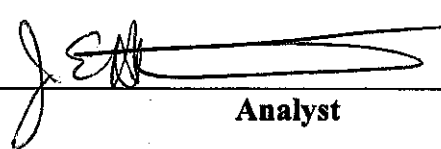
Exp Date: 12/18/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 10:48am |
| AIR BLK  | .00    | 10:49am |
| ACCY CHK | .07    | 10:49am |
| AIR BLK  | .00    | 10:50am |
| SUB TEST | .00    | 10:51am |
| AIR BLK  | .00    | 10:52am |
| SUB TEST | .00    | 10:53am |
| AIR BLK  | .00    | 10:54am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007



**Intox EC/IR-II: Preventive Maintenance**

GASTON COUNTY GASTON COUNTY SD 350

Serial Number: 008643      Test Record Number: 2055  
Test Date: 01/23/2015      Test Time: 10:59am EST

System Check: Passed

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:00am |
| FLO  | Pass   | 11:00am |
| FC   | Pass   | 11:00am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:00am |
| SRC  | Pass   | 11:00am |
| DET  | Pass   | 11:00am |
| BAR  | Pass   | 11:00am |
| BT   | Pass   | 11:00am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:00am |

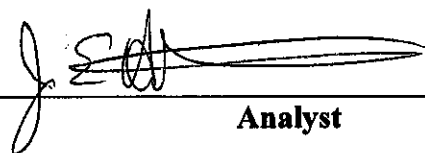
**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:00am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:01am |
| CAL  | Pass   | 11:01am |

Preventive Maintenance  
Status: Pass

  
\_\_\_\_\_  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II

County Catawba Instrument Location Catawba County SD  
Instrument Serial No. 008687 100 B Southwest Blvd, Newton  
828-464-5271

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 23<sup>rd</sup> day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Joseph E. Hatcher  
Signature of Certifying Official

654  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

CATAWBA COUNTY CATAWBA COUNTY SD 170

Serial Number: 008687

Test Date: 01/23/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: HUTCHINSON, JOSEPH E

Permit Number: 19951E

Effective:

10/01/2013-10/01/2015

Officer's Name: NONE, NONE

Type of Agency: FTA

Agency: DHHS


Test Type: Breath Test

Lot Number: AG322601

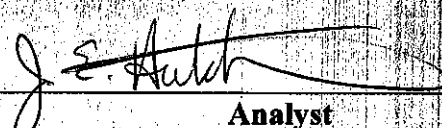
Exp Date: 08/14/2015

| Test     | g/210L | Time   |
|----------|--------|--------|
| DIAG     | Pass   | 9:38am |
| AIR BLK  | .00    | 9:39am |
| ACCY CHK | .07    | 9:40am |
| AIR BLK  | .00    | 9:41am |
| SUB TEST | .00    | 9:42am |
| AIR BLK  | .00    | 9:43am |
| SUB TEST | .00    | 9:44am |
| AIR BLK  | .00    | 9:45am |

Reported AC: .00 g/210L

  
Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

CATAWBA COUNTY CATAWBA COUNTY SD 170

Serial Number: 008687      Test Record Number: 1986  
Test Date: 01/23/2015      Test Time: 9:46am EST

**System Check: Passed**

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 9:47am |
| FLO  | Pass   | 9:47am |
| FC   | Pass   | 9:47am |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 9:47am |
| SRC  | Pass   | 9:47am |
| DET  | Pass   | 9:47am |
| BAR  | Pass   | 9:47am |
| BT   | Pass   | 9:47am |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 9:47am |

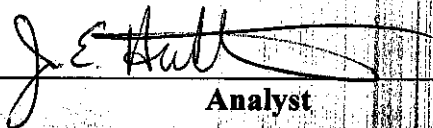
**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 9:47am |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 9:48am |
| CAL  | Pass   | 9:48am |

**Preventive Maintenance**  
Status: Pass

  
Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Swain Instrument Location Cherokee PD  
Instrument Serial No. 008782 Cherokee, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 27 day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



Chris R. Cuth  
Signature of Certifying Official

635  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

SWAIN COUNTY CHEROKEE INDIAN PD 860

Serial Number: 008782

Test Date: 01/27/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R

Permit Number: 8457E

Effective:

10/01/2013-10/01/2015

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG335201


Exp Date: 12/18/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:19am |
| AIR BLK  | .00    | 11:19am |
| ACCY CHK | .07    | 11:20am |
| AIR BLK  | .00    | 11:21am |
| SUB TEST | .00    | 11:22am |
| AIR BLK  | .00    | 11:23am |
| SUB TEST | .00    | 11:24am |
| AIR BLK  | .00    | 11:25am |

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

Intox EC/IR-II: Preventive Maintenance

SWAIN COUNTY CHEROKEE INDIAN PD 860

Serial Number: 008782 Test Record Number: 853

Test Date: 01/27/2015 Test Time: 11:26am EST

System Check: *Passed*

Baseline Tests

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:26am |
| FLO  | Pass   | 11:26am |
| FC   | Pass   | 11:26am |

Temperature Tests

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:26am |
| SRC  | Pass   | 11:26am |
| DET  | Pass   | 11:26am |
| BAR  | Pass   | 11:26am |
| BT   | Pass   | 11:26am |

Blank Tests

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:27am |

Printer Tests


| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:27am |

CRC Tests

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:27am |
| CAL  | Pass   | 11:27am |

Preventive Maintenance

Status: Pass



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Clay Instrument Location Clay Co. Jail  
Instrument Serial No. 008608 Hayesville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 26 day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David K. Cuthbert  
Signature of Certifying Official

635  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.



**Intox EC/IR-II: Subject Test**

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608  
Test Date: 01/26/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R

Permit Number: 8457E

Effective:

10/01/2013-10/01/2015

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG335201


Exp Date: 12/18/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:45am |
| AIR BLK  | .00    | 11:45am |
| ACCY CHK | .07    | 11:46am |
| AIR BLK  | .00    | 11:47am |
| SUB TEST | .00    | 11:48am |
| AIR BLK  | .00    | 11:48am |
| SUB TEST | .00    | 11:50am |
| AIR BLK  | .00    | 11:51am |

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

  
Analyst

Intox EC/IR-II: Preventive Maintenance

CLAY COUNTY CLAY COUNTY JAIL 210

Serial Number: 008608 Test Record Number: 1049  
Test Date: 01/26/2015 Test Time: 11:51am EST

System Check: Passed

Baseline Tests

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:52am |
| FLO  | Pass   | 11:52am |
| FC   | Pass   | 11:52am |

Temperature Tests

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:52am |
| SRC  | Pass   | 11:52am |
| DET  | Pass   | 11:52am |
| BAR  | Pass   | 11:52am |
| BT   | Pass   | 11:52am |

Blank Tests

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:53am |


Printer Tests

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:53am |

CRC Tests

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:53am |
| CAL  | Pass   | 11:53am |

Preventive Maintenance  
Status: Pass



Analyst

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Graham Instrument Location Graham Co. S.O.  
Instrument Serial No. 008915 Robbinsville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 20 day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cutler  
Signature of Certifying Official

635  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

GRAHAM COUNTY GRAHAM COUNTY SD 370

Serial Number: 008915

Test Date: 01/20/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R

Permit Number: 8457E

Effective:

10/01/2013-10/01/2015

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG326006

Exp Date: 09/17/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:27am |
| AIR BLK  | .00    | 11:28am |
| ACCY CHK | .08    | 11:29am |
| AIR BLK  | .00    | 11:30am |
| SUB TEST | .00    | 11:30am |
| AIR BLK  | .00    | 11:31am |
| SUB TEST | .00    | 11:33am |
| AIR BLK  | .00    | 11:34am |

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR

  
Analyst

**Intox EC/IR-II: Preventive Maintenance**

**GRAHAM COUNTY GRAHAM COUNTY SD 370**

Serial Number: 008915      Test Record Number: 617  
Test Date: 01/20/2015      Test Time: 11:35am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:35am |
| FLO  | Pass   | 11:35am |
| FC   | Pass   | 11:35am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:35am |
| SRC  | Pass   | 11:35am |
| DET  | Pass   | 11:35am |
| BAR  | Pass   | 11:35am |
| BT   | Pass   | 11:35am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:36am |


**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:36am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:36am |
| CAL  | Pass   | 11:36am |

Preventive Maintenance  
Status: Pass



**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Jackson Instrument Location Jackson Co Jail  
Instrument Serial No. 008722 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Luth  
Signature of Certifying Official

635  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

Intox EC/IR-II: Subject Test

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008722

Test Date: 01/08/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R

Permit Number: 8457E

Effective:

10/01/2013-10/01/2015

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG335201


Exp Date: 12/18/2015

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:14am |
| AIR BLK  | .00    | 11:15am |
| ACCY CHK | .07    | 11:15am |
| AIR BLK  | .00    | 11:17am |
| SUB TEST | .00    | 11:17am |
| AIR BLK  | .00    | 11:18am |
| SUB TEST | .00    | 11:19am |
| AIR BLK  | .00    | 11:20am |

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

This form is used when performing Preventive Maintenance procedures

Forensic Tests for Alcohol Branch

Department of Health and Human Services

Rev. 12/2007

**Intox EC/IR-II: Preventive Maintenance**

**JACKSON COUNTY JACKSON COUNTY JAIL 490**

Serial Number: 008722      Test Record Number: 654  
Test Date: 01/08/2015      Test Time: 11:21am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:22am |
| FLO  | Pass   | 11:22am |
| FC   | Pass   | 11:22am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:22am |
| SRC  | Pass   | 11:22am |
| DET  | Pass   | 11:22am |
| BAR  | Pass   | 11:22am |
| BT   | Pass   | 11:22am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:23am |


**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:23am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:23am |
| CAL  | Pass   | 11:23am |

Preventive Maintenance  
Status: Pass



**Analyst**



DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Jackson Instrument Location Jackson Co. Jail  
Instrument Serial No. 008708 Sylva, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 8 day of January, 20 15 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



David R. Cuth

Signature of Certifying Official

635

Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

JACKSON COUNTY JACKSON COUNTY JAIL 490

Serial Number: 008708

Test Date: 01/08/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: CUTLER, DANIEL R

Permit Number: 8457E

Effective:

10/01/2013-10/01/2015

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG409709


Exp Date: 04/07/2016

| Test     | g/210L | Time    |
|----------|--------|---------|
| DIAG     | Pass   | 11:12am |
| AIR BLK  | .00    | 11:13am |
| ACCY CHK | .08    | 11:13am |
| AIR BLK  | .00    | 11:14am |
| SUB TEST | .00    | 11:15am |
| AIR BLK  | .00    | 11:16am |
| SUB TEST | .00    | 11:17am |
| AIR BLK  | .00    | 11:18am |

Reported AC: .00 g/210L

Signature of Chemical Analyst

Court CVR



Analyst

**This form is used when performing Preventive Maintenance procedures**

**Forensic Tests for Alcohol Branch**

**Department of Health and Human Services**

**Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

**JACKSON COUNTY JACKSON COUNTY JAIL 490**

Serial Number: 008708      Test Record Number: 1032  
Test Date: 01/08/2015      Test Time: 11:20am EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time    |
|------|--------|---------|
| IR   | Pass   | 11:20am |
| FLO  | Pass   | 11:20am |
| FC   | Pass   | 11:20am |

**Temperature Tests**

| Test | Status | Time    |
|------|--------|---------|
| FC1  | Pass   | 11:21am |
| SRC  | Pass   | 11:21am |
| DET  | Pass   | 11:21am |
| BAR  | Pass   | 11:21am |
| BT   | Pass   | 11:21am |

**Blank Tests**

| Test | Status | Time    |
|------|--------|---------|
| AIR  | Pass   | 11:21am |


**Printer Tests**

| Test | Status | Time    |
|------|--------|---------|
| PRNT | Pass   | 11:21am |

**CRC Tests**

| Test | Status | Time    |
|------|--------|---------|
| COMP | Pass   | 11:21am |
| CAL  | Pass   | 11:21am |

Preventive Maintenance  
Status: Pass



**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH

**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**


County Henderson Instrument Location Henderson Co. Detention

Instrument Serial No. 008822 Hendersonville, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 7 day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



  
Signature of Certifying Official

649  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

**HENDERSON COUNTY DETENTION 440**

Serial Number: 008822

Test Date: 01/07/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

06/01/2013-06/01/2015

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG326006

Exp Date: 09/17/2015

| Test            | g/210L     | Time          |
|-----------------|------------|---------------|
| DIAG            | Pass       | 4:10pm        |
| AIR BLK         | .00        | 4:11pm        |
| ACCY CHK        | .08        | 4:12pm        |
| AIR BLK         | .00        | 4:13pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>4:14pm</b> |
| AIR BLK         | .00        | 4:15pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>4:16pm</b> |
| AIR BLK         | .00        | 4:17pm        |

**Reported AC: .00 g/210L**

\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**

**Intox EC/IR-II: Preventive Maintenance**

**HENDERSON COUNTY DETENTION 440**

Serial Number: 008822      Test Record Number: 1747  
Test Date: 01/07/2015      Test Time: 4:18pm EST

System Check: Passed

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 4:18pm |
| FLO  | Pass   | 4:19pm |
| FC   | Pass   | 4:19pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 4:19pm |
| SRC  | Pass   | 4:19pm |
| DET  | Pass   | 4:19pm |
| BAR  | Pass   | 4:19pm |
| BT   | Pass   | 4:19pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 4:19pm |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 4:19pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 4:20pm |
| CAL  | Pass   | 4:20pm |

Preventive Maintenance  
Status: Pass

  
**Analyst**

DEPARTMENT OF HEALTH AND HUMAN SERVICES  
FORENSIC TESTS FOR ALCOHOL BRANCH


**PREVENTIVE MAINTENANCE RECORD  
INTOXIMETERS, MODEL INTOX EC/IR II**

County Watauga Instrument Location Watauga Co. Jail  
Instrument Serial No. 008715 Boone, NC

The preventive maintenance procedures for the Intoximeters, Model Intox EC/IR II to be followed at least once every four months are:

1. Verify the ethanol gas canister displays pressure, or the alcoholic breath simulator thermometer shows 34 degrees, plus or minus .2 degree centigrade;
2. Verify instrument displays time and date;
3. Initiate breath test sequence;
4. Enter information as prompted;
5. Verify instrument accuracy;
6. When "PLEASE BLOW" appears, collect breath sample;
7. When "PLEASE BLOW" appears, collect breath sample;
8. Print test record;
9. Verify Diagnostic Program; and
10. Verify that the ethanol gas canister is being changed before expiration date, or the alcoholic breath simulator solution is being changed every four months or after 125 Alcoholic Breath Simulator tests, whichever occurs first.

I certify that on the 13 day of January, 2015 the forgoing preventive maintenance procedures were performed on the instrument indicated above, in accordance with current regulations of the N.C. Department of Health and Human Services, and the instrument is functioning properly.



[Signature]  
Signature of Certifying Official

649  
Certificate Number

A signed original of the preventive maintenance record shall be kept on file for at least three years.

**Intox EC/IR-II: Subject Test**

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008715

Test Date: 01/13/2015

Citation Number: M0000000-0

Subject's Name:

PREVENTIVE, MAINTENANCE

Subject's Date of Birth: 11/11/1911

Subject's Sex: Male

Driver's License State: XX

Driver's License Number: NONE

Analyst's Name: BURNETTE, ANTHONY J

Permit Number: 11304E

Effective:

06/01/2013-06/01/2015

Officer's Name: NONE,

Type of Agency: FTA

Agency: DHHS

Test Type: Breath Test

Lot Number: AG405702

Exp Date: 02/26/2016

| Test            | g/210L     | Time          |
|-----------------|------------|---------------|
| DIAG            | Pass       | 1:19pm        |
| AIR BLK         | .00        | 1:20pm        |
| ACCY CHK        | .08        | 1:21pm        |
| AIR BLK         | .00        | 1:22pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>1:23pm</b> |
| AIR BLK         | .00        | 1:24pm        |
| <b>SUB TEST</b> | <b>.00</b> | <b>1:25pm</b> |
| AIR BLK         | .00        | 1:26pm        |

Reported AC: .00 g/210L

\_\_\_\_\_  
Signature of Chemical Analyst

Court CVR

  
\_\_\_\_\_  
Analyst

**This form is used when performing Preventive Maintenance procedures  
Forensic Tests for Alcohol Branch  
Department of Health and Human Services  
Rev. 12/2007**



**Intox EC/IR-II: Preventive Maintenance**

WATAUGA COUNTY WATAUGA JAIL 940

Serial Number: 008715      Test Record Number: 1581  
Test Date: 01/13/2015      Test Time: 1:32pm EST

System Check: *Passed*

**Baseline Tests**

| Test | Status | Time   |
|------|--------|--------|
| IR   | Pass   | 1:32pm |
| FLO  | Pass   | 1:32pm |
| FC   | Pass   | 1:33pm |

**Temperature Tests**

| Test | Status | Time   |
|------|--------|--------|
| FC1  | Pass   | 1:33pm |
| SRC  | Pass   | 1:33pm |
| DET  | Pass   | 1:33pm |
| BAR  | Pass   | 1:33pm |
| BT   | Pass   | 1:33pm |

**Blank Tests**

| Test | Status | Time   |
|------|--------|--------|
| AIR  | Pass   | 1:33pm |

**Printer Tests**

| Test | Status | Time   |
|------|--------|--------|
| PRNT | Pass   | 1:33pm |

**CRC Tests**

| Test | Status | Time   |
|------|--------|--------|
| COMP | Pass   | 1:34pm |
| CAL  | Pass   | 1:34pm |

Preventive Maintenance  
Status: Pass

  
**Analyst**